

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035315.D
 Acq On : 19 Apr 2024 18:01
 Operator : SY/MD
 Sample : P2157-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	187496	198844	12.70%	1.681%
2	1.529	146	152	167	rVB	168772	196954	12.58%	1.665%
3	2.056	308	316	329	rVB	316701	449789	28.72%	3.802%
4	2.442	430	436	450	rVB6	1991	3739	0.24%	0.032%
5	2.667	505	506	510	rBV2	239	124	0.01%	0.001%
6	2.738	525	528	530	rBV	382	268	0.02%	0.002%
7	2.960	592	597	598	rBV2	347	279	0.02%	0.002%
8	3.021	614	616	618	rBV	238	174	0.01%	0.001%
9	3.053	621	626	627	rBV	415	325	0.02%	0.003%
10	3.089	634	637	638	rBV2	345	213	0.01%	0.002%
11	3.117	644	646	651	rVB3	229	144	0.01%	0.001%
12	3.159	657	659	663	rBV3	280	162	0.01%	0.001%
13	3.208	672	674	677	rVB	335	154	0.01%	0.001%
14	3.227	677	680	681	rBV	180	96	0.01%	0.001%
15	3.253	685	688	691	rBV	265	173	0.01%	0.001%
16	3.307	703	705	706	rBV	245	111	0.01%	0.001%
17	3.355	717	720	721	rBV	198	107	0.01%	0.001%
18	3.365	721	723	725	rVV	414	192	0.01%	0.002%
19	3.400	731	734	735	rBV	234	110	0.01%	0.001%
20	3.439	743	746	750	rBV	293	295	0.02%	0.002%
21	3.481	755	759	761	rBV2	163	142	0.01%	0.001%
22	3.519	769	771	778	rVB3	201	189	0.01%	0.002%
23	3.548	778	780	781	rBV2	151	60	0.00%	0.001%
24	3.558	781	783	786	rVB	191	88	0.01%	0.001%
25	3.606	794	798	800	rBV	269	175	0.01%	0.001%
26	3.651	809	812	816	rVB	444	256	0.02%	0.002%
27	3.674	816	819	822	rBV	541	335	0.02%	0.003%
28	3.786	845	854	896	rBV	114690	344100	21.97%	2.908%
29	4.246	983	997	1031	rBV	248467	631912	40.35%	5.341%
30	4.851	1182	1185	1186	rBV	214	100	0.01%	0.001%
31	4.953	1202	1217	1261	rBV2	592336	1565988	100.00%	13.236%
32	5.404	1355	1357	1361	rVB2	363	202	0.01%	0.002%
33	5.420	1361	1362	1363	rBV2	194	57	0.00%	0.000%
34	5.449	1369	1371	1373	rBV	590	390	0.02%	0.003%
35	5.532	1386	1397	1436	rBV	440141	931006	59.45%	7.869%
36	5.834	1481	1491	1503	rBV5	6681	14616	0.93%	0.124%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035315.D
 Acq On : 19 Apr 2024 18:01
 Operator : SY/MD
 Sample : P2157-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1573	rBV	349037	726773	46.41%	6.143%
38	6.291	1629	1633	1637	rVB4	436	389	0.02%	0.003%
39	6.323	1637	1643	1644	rBV2	676	571	0.04%	0.005%
40	6.355	1651	1653	1654	rBV	259	136	0.01%	0.001%
41	6.381	1659	1661	1664	rBV	452	255	0.02%	0.002%
42	6.416	1669	1672	1678	rVB5	513	577	0.04%	0.005%
43	6.445	1678	1681	1683	rBV2	268	151	0.01%	0.001%
44	6.465	1683	1687	1692	rVV3	574	506	0.03%	0.004%
45	6.490	1692	1695	1700	rVV2	500	473	0.03%	0.004%
46	6.510	1700	1701	1704	rVV	440	168	0.01%	0.001%
47	6.539	1708	1710	1714	rVB2	421	264	0.02%	0.002%
48	6.584	1722	1724	1725	rVB2	248	64	0.00%	0.001%
49	6.593	1725	1727	1728	rBV	358	116	0.01%	0.001%
50	6.645	1741	1743	1747	rVB3	482	262	0.02%	0.002%
51	6.783	1784	1786	1791	rBV4	308	191	0.01%	0.002%
52	6.834	1799	1802	1804	rBV2	100	69	0.00%	0.001%
53	6.850	1804	1807	1809	rBV	184	116	0.01%	0.001%
54	6.912	1816	1826	1849	rBV	147214	290143	18.53%	2.452%
55	7.243	1918	1929	1964	rBV	644890	1149810	73.42%	9.718%
56	7.555	2016	2026	2053	rBV	102382	200138	12.78%	1.692%
57	7.969	2152	2155	2157	rBV2	311	163	0.01%	0.001%
58	8.024	2163	2172	2208	rBV2	336275	737698	47.11%	6.235%
59	8.638	2361	2363	2365	rVB	390	171	0.01%	0.001%
60	8.664	2368	2371	2372	rBV	283	148	0.01%	0.001%
61	8.706	2381	2384	2387	rBV	416	328	0.02%	0.003%
62	8.783	2397	2408	2436	rBV	705845	1212346	77.42%	10.247%
63	9.137	2516	2518	2520	rVB3	553	275	0.02%	0.002%
64	9.223	2543	2545	2547	rBV	312	132	0.01%	0.001%
65	9.239	2547	2550	2554	rVV3	480	270	0.02%	0.002%
66	9.301	2567	2569	2571	rBV	301	154	0.01%	0.001%
67	9.400	2599	2600	2603	rBV2	253	123	0.01%	0.001%
68	9.545	2639	2645	2647	rBV3	369	360	0.02%	0.003%
69	9.571	2650	2653	2655	rBV2	181	127	0.01%	0.001%
70	9.651	2674	2678	2680	rBV3	265	207	0.01%	0.002%
71	9.712	2696	2697	2699	rBV3	231	110	0.01%	0.001%
72	9.825	2729	2732	2735	rBV2	343	221	0.01%	0.002%
73	9.837	2735	2736	2738	rVV2	190	62	0.00%	0.001%
74	9.905	2754	2757	2759	rBV	408	229	0.01%	0.002%
75	9.918	2759	2761	2763	rVB2	177	55	0.00%	0.000%
76	9.960	2769	2774	2779	rBV3	468	512	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035315.D
 Acq On : 19 Apr 2024 18:01
 Operator : SY/MD
 Sample : P2157-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCOR80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.992	2782	2784	2786	rBV	377	168	0.01%	0.001%
78	10.011	2786	2790	2793	rVB	354	231	0.01%	0.002%
79	10.030	2794	2796	2798	rBV2	408	191	0.01%	0.002%
80	10.149	2821	2833	2864	rBV	526152	835165	53.33%	7.059%
81	10.419	2916	2917	2919	rVB	183	69	0.00%	0.001%
82	10.564	2957	2962	2966	rBV	241	216	0.01%	0.002%
83	10.593	2968	2971	2972	rBV2	293	144	0.01%	0.001%
84	10.712	3003	3008	3011	rBV2	405	331	0.02%	0.003%
85	10.831	3042	3045	3050	rBV2	288	227	0.01%	0.002%
86	10.863	3054	3055	3056	rBV	181	57	0.00%	0.000%
87	10.998	3096	3097	3100	rBV	214	102	0.01%	0.001%
88	11.021	3100	3104	3106	rBV2	307	204	0.01%	0.002%
89	11.130	3130	3138	3144	rBV4	3763	5285	0.34%	0.045%
90	11.185	3144	3155	3186	rVV	671577	1080856	69.02%	9.136%
91	11.500	3242	3253	3260	rBV4	11559	24100	1.54%	0.204%
92	11.558	3261	3271	3296	rVB	710839	1149156	73.38%	9.713%
93	11.828	3352	3355	3356	rBV3	584	341	0.02%	0.003%
94	12.188	3465	3467	3468	rBV	523	234	0.01%	0.002%
95	12.799	3655	3657	3660	rBV2	331	165	0.01%	0.001%
96	12.879	3679	3682	3685	rBV3	418	281	0.02%	0.002%
97	13.040	3730	3732	3735	rBV	413	243	0.02%	0.002%
98	13.201	3773	3782	3799	rBV2	31010	49766	3.18%	0.421%
99	13.532	3883	3885	3886	rBV	438	184	0.01%	0.002%
100	13.683	3924	3932	3949	rBV3	10366	16702	1.07%	0.141%




Sum of corrected areas: 11831150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035315.D
Acq On : 19 Apr 2024 18:01
Operator : SY/MD
Sample : P2157-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

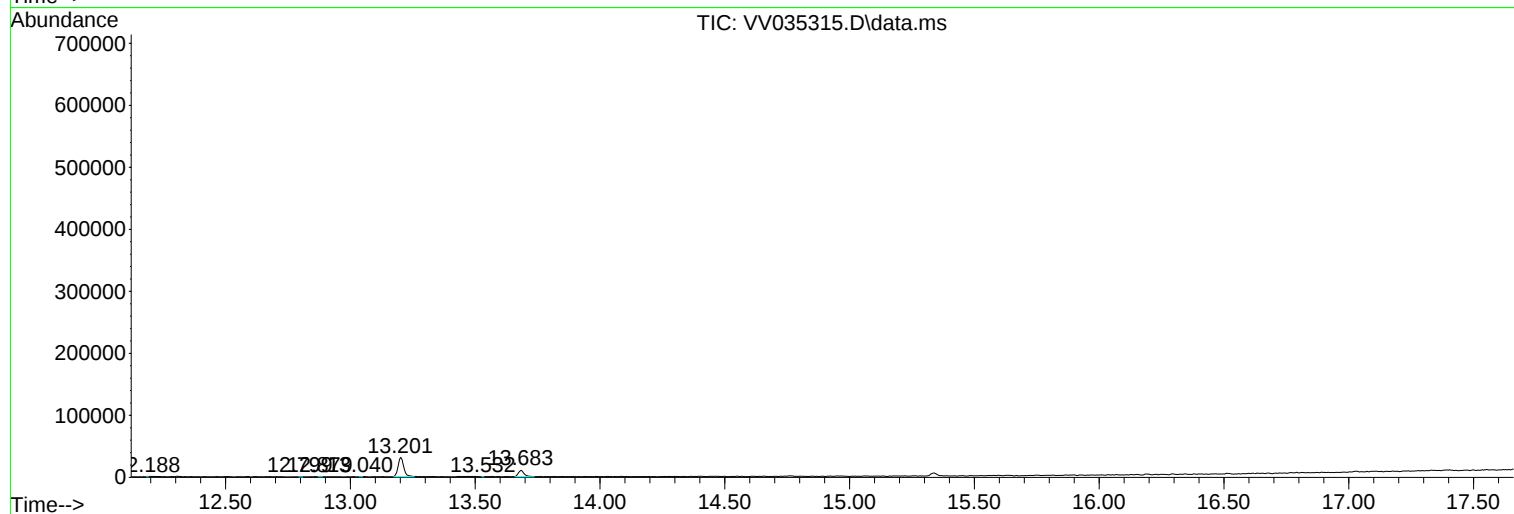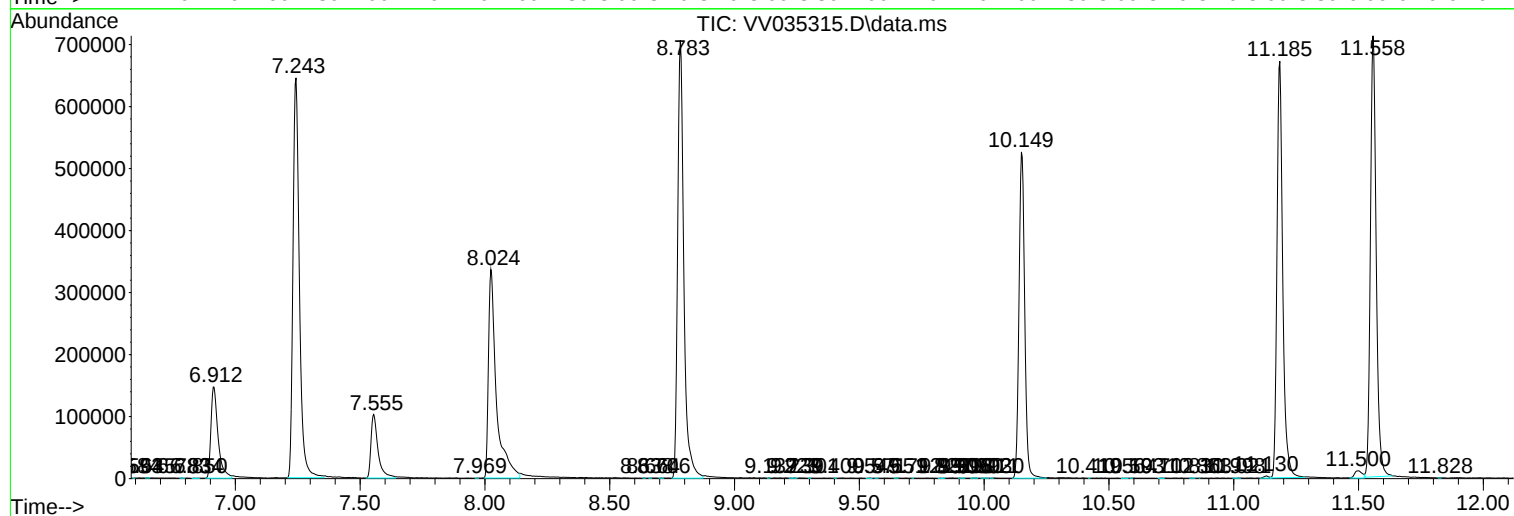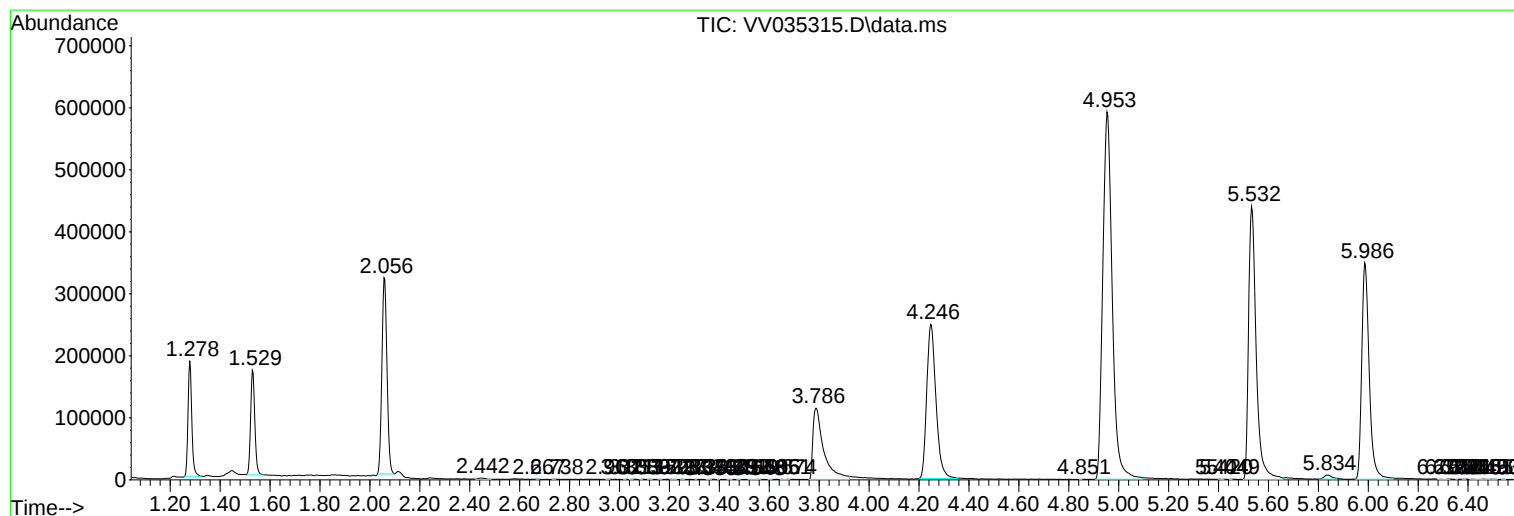

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035315.D
Acq On : 19 Apr 2024 18:01
Operator : SY/MD
Sample : P2157-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035315.D
Acq On : 19 Apr 2024 18:01
Operator : SY/MD
Sample : P2157-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------