

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035316.D
 Acq On : 19 Apr 2024 18:24
 Operator : SY/MD
 Sample : VIBLK279
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rBV	171253	179610	11.84%	1.552%
2	1.529	146	152	168	rVB	159795	189949	12.52%	1.641%
3	2.060	308	317	336	rVB	301228	439665	28.97%	3.798%
4	2.519	458	460	463	rBV2	436	334	0.02%	0.003%
5	2.561	471	473	478	rBV3	358	230	0.02%	0.002%
6	2.616	488	490	492	rBV	329	196	0.01%	0.002%
7	2.822	552	554	555	rBV	230	91	0.01%	0.001%
8	2.902	577	579	580	rBV	236	114	0.01%	0.001%
9	2.934	586	589	592	rVB2	348	214	0.01%	0.002%
10	2.969	596	600	602	rVV2	415	308	0.02%	0.003%
11	2.992	605	607	611	rVB2	316	177	0.01%	0.002%
12	3.037	618	621	624	rBV	366	265	0.02%	0.002%
13	3.121	645	647	650	rBV2	340	167	0.01%	0.001%
14	3.182	663	666	667	rBV2	233	138	0.01%	0.001%
15	3.211	671	675	676	rBV	314	210	0.01%	0.002%
16	3.285	695	698	700	rBV	197	124	0.01%	0.001%
17	3.297	700	702	704	rVB	364	126	0.01%	0.001%
18	3.320	708	709	715	rVB2	220	165	0.01%	0.001%
19	3.352	715	719	722	rBV3	267	262	0.02%	0.002%
20	3.416	736	739	741	rBV3	285	213	0.01%	0.002%
21	3.429	741	743	745	rVV2	348	143	0.01%	0.001%
22	3.458	749	752	756	rVB2	189	168	0.01%	0.001%
23	3.638	805	808	810	rBV2	209	173	0.01%	0.001%
24	3.658	810	814	817	rVV2	305	302	0.02%	0.003%
25	3.686	821	823	826	rVB2	379	195	0.01%	0.002%
26	3.786	846	854	901	rBV	120987	352876	23.25%	3.049%
27	4.246	983	997	1037	rBV	243452	628990	41.45%	5.434%
28	4.587	1101	1103	1108	rBV3	372	251	0.02%	0.002%
29	4.953	1202	1217	1264	rBV2	568320	1517557	100.00%	13.110%
30	5.384	1349	1351	1355	rVB2	416	230	0.02%	0.002%
31	5.532	1386	1397	1428	rBV	433355	917497	60.46%	7.926%
32	5.985	1526	1538	1562	rBV	339803	710759	46.84%	6.140%
33	6.339	1645	1648	1652	rVB3	457	301	0.02%	0.003%
34	6.365	1653	1656	1659	rVB2	441	258	0.02%	0.002%
35	6.381	1659	1661	1663	rBV	399	187	0.01%	0.002%
36	6.403	1666	1668	1671	rVB	355	183	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035316.D
 Acq On : 19 Apr 2024 18:24
 Operator : SY/MD
 Sample : VIBLK279
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.429	1673	1676	1680	rBV5	555	410	0.03%	0.004%
38	6.510	1697	1701	1702	rBV	561	240	0.02%	0.002%
39	6.526	1705	1706	1709	rVB	355	141	0.01%	0.001%
40	6.574	1717	1721	1724	rBV2	172	155	0.01%	0.001%
41	6.622	1732	1736	1737	rBV2	420	272	0.02%	0.002%
42	6.690	1754	1757	1759	rBV2	259	174	0.01%	0.002%
43	6.809	1792	1794	1798	rBV	195	117	0.01%	0.001%
44	6.873	1809	1814	1817	rBV	308	287	0.02%	0.002%
45	6.911	1817	1826	1857	rBV	155758	307165	20.24%	2.654%
46	7.243	1918	1929	1974	rBV	623307	1114532	73.44%	9.629%
47	7.554	2017	2026	2054	rBV	108825	204099	13.45%	1.763%
48	7.815	2103	2107	2109	rBV2	339	219	0.01%	0.002%
49	7.902	2131	2134	2135	rBV2	208	116	0.01%	0.001%
50	7.937	2143	2145	2147	rBV2	382	203	0.01%	0.002%
51	8.024	2163	2172	2222	rBV	342558	766196	50.49%	6.619%
52	8.545	2331	2334	2335	rBV2	565	287	0.02%	0.002%
53	8.648	2364	2366	2370	rBV3	339	185	0.01%	0.002%
54	8.706	2382	2384	2388	rVB2	472	294	0.02%	0.003%
55	8.731	2388	2392	2394	rBV2	429	299	0.02%	0.003%
56	8.783	2397	2408	2443	rBV	697228	1181063	77.83%	10.203%
57	9.140	2515	2519	2522	rBV2	414	400	0.03%	0.003%
58	9.242	2550	2551	2554	rVB	352	145	0.01%	0.001%
59	9.262	2554	2557	2559	rBV2	341	174	0.01%	0.002%
60	9.304	2567	2570	2571	rBV	245	107	0.01%	0.001%
61	9.345	2581	2583	2585	rBV	241	120	0.01%	0.001%
62	9.429	2606	2609	2611	rBV2	143	91	0.01%	0.001%
63	9.445	2611	2614	2616	rVV2	377	187	0.01%	0.002%
64	9.477	2620	2624	2628	rBV3	264	252	0.02%	0.002%
65	9.500	2628	2631	2632	rBV2	270	179	0.01%	0.002%
66	9.548	2642	2646	2650	rBV	284	233	0.02%	0.002%
67	9.570	2650	2653	2655	rBV	201	112	0.01%	0.001%
68	9.628	2668	2671	2676	rVB2	444	265	0.02%	0.002%
69	9.680	2682	2687	2689	rBV3	306	282	0.02%	0.002%
70	9.738	2702	2705	2708	rBV	245	196	0.01%	0.002%
71	9.757	2709	2711	2713	rBV3	270	146	0.01%	0.001%
72	9.802	2722	2725	2727	rBV	286	146	0.01%	0.001%
73	9.873	2745	2747	2749	rBV	198	92	0.01%	0.001%
74	9.886	2749	2751	2754	rVV	231	144	0.01%	0.001%
75	9.947	2767	2770	2774	rBV3	254	228	0.02%	0.002%
76	9.995	2781	2785	2789	rVB2	316	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035316.D
 Acq On : 19 Apr 2024 18:24
 Operator : SY/MD
 Sample : VIBLK279
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK279

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.024	2792	2794	2797	rVB	244	121	0.01%	0.001%
78	10.149	2821	2833	2859	rBV	526491	846023	55.75%	7.309%
79	10.419	2915	2917	2920	rVB2	333	186	0.01%	0.002%
80	10.442	2920	2924	2928	rBV3	217	197	0.01%	0.002%
81	10.796	3030	3034	3041	rVB4	652	667	0.04%	0.006%
82	10.844	3046	3049	3050	rBV2	285	160	0.01%	0.001%
83	10.879	3056	3060	3064	rBV3	425	372	0.02%	0.003%
84	10.924	3071	3074	3076	rBV	251	132	0.01%	0.001%
85	10.969	3086	3088	3092	rVB	285	126	0.01%	0.001%
86	11.040	3108	3110	3116	rVB3	474	393	0.03%	0.003%
87	11.072	3116	3120	3123	rVB2	314	276	0.02%	0.002%
88	11.101	3126	3129	3131	rBV	190	110	0.01%	0.001%
89	11.127	3133	3137	3141	rBV5	1329	1561	0.10%	0.013%
90	11.185	3144	3155	3178	rBV	674126	1063214	70.06%	9.185%
91	11.558	3260	3271	3298	rBV	709953	1114489	73.44%	9.628%
92	12.188	3462	3467	3469	rBV2	475	418	0.03%	0.004%
93	12.316	3504	3507	3509	rBV	184	130	0.01%	0.001%
94	12.557	3578	3582	3585	rBV3	562	442	0.03%	0.004%
95	12.972	3707	3711	3714	rVB2	329	211	0.01%	0.002%
96	13.078	3741	3744	3748	rBV3	385	315	0.02%	0.003%
97	13.204	3775	3783	3800	rVB3	10500	17429	1.15%	0.151%
98	13.461	3860	3863	3866	rBV4	599	456	0.03%	0.004%
99	13.635	3915	3917	3922	rBV3	615	376	0.02%	0.003%
100	13.686	3927	3933	3946	rVB7	2947	4743	0.31%	0.041%




Sum of corrected areas: 11575323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035316.D
Acq On : 19 Apr 2024 18:24
Operator : SY/MD
Sample : VIBLK279
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

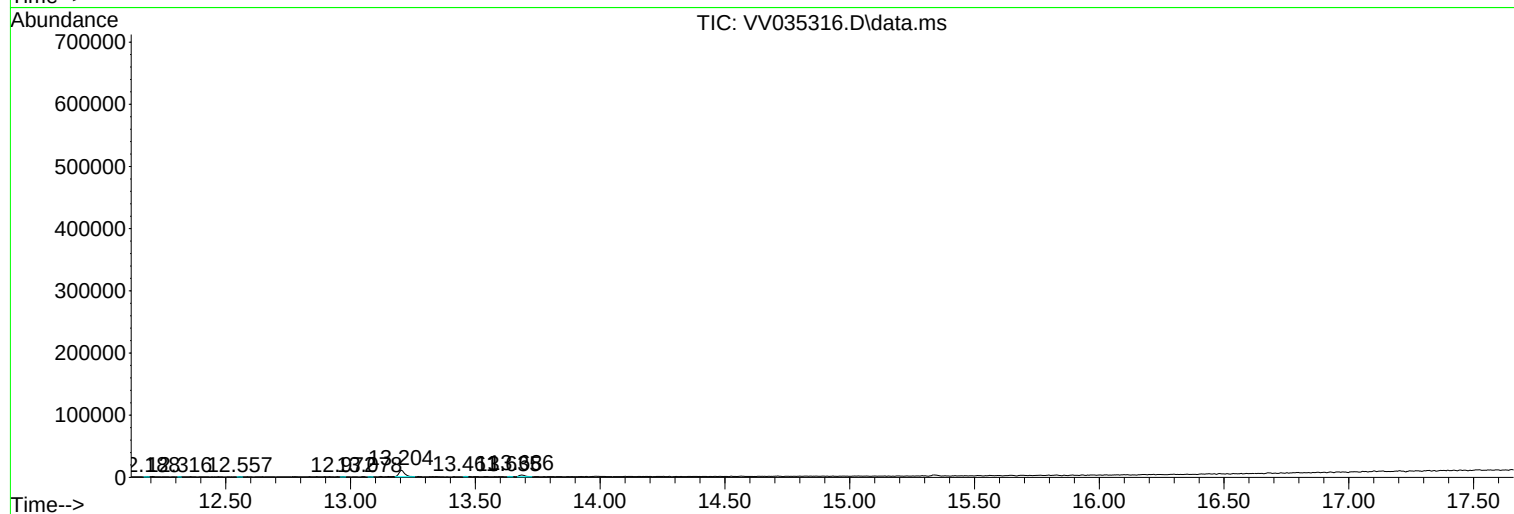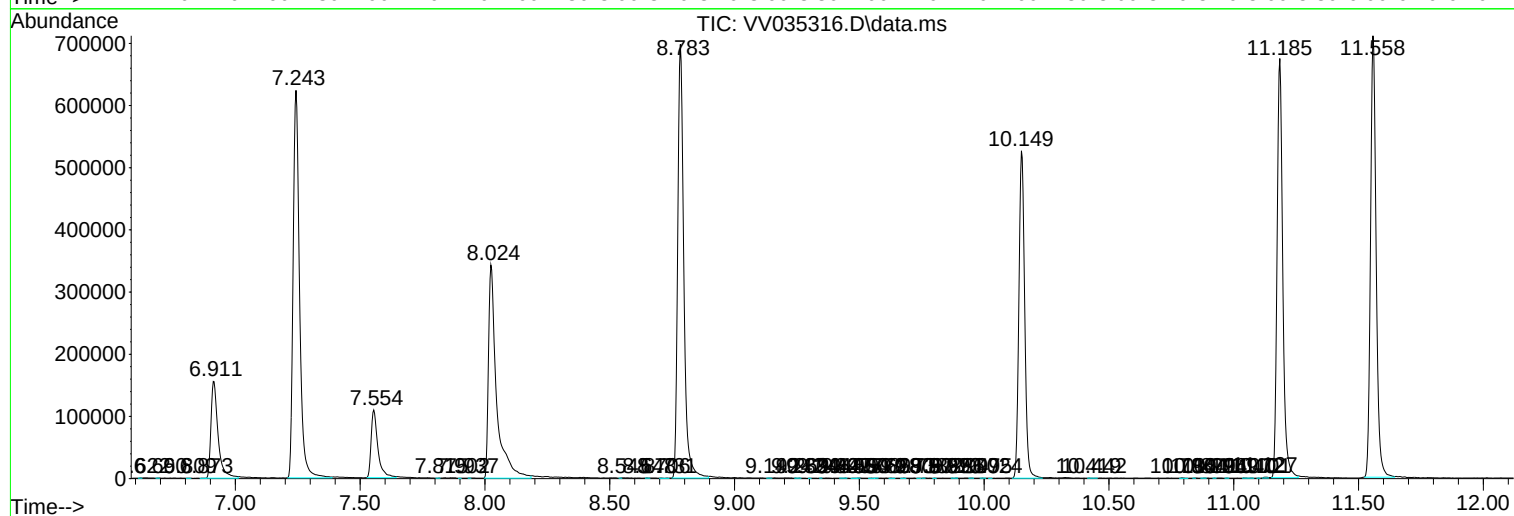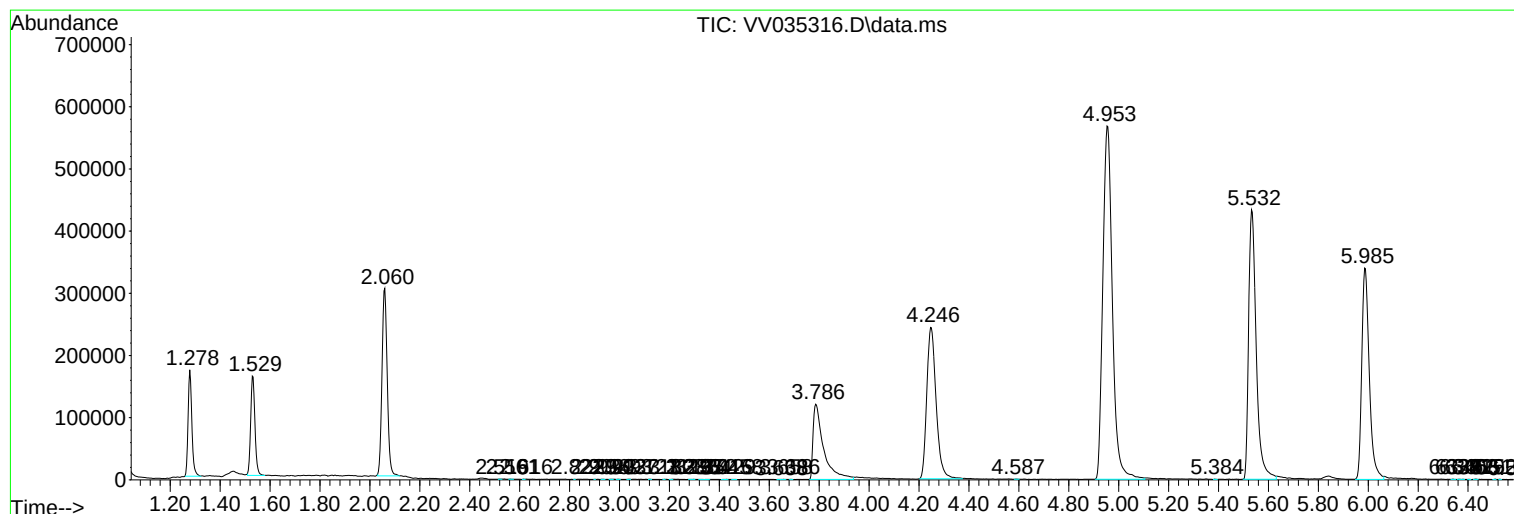

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035316.D
Acq On : 19 Apr 2024 18:24
Operator : SY/MD
Sample : VIBLK279
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035316.D
Acq On : 19 Apr 2024 18:24
Operator : SY/MD
Sample : VIBLK279
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK279

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------