

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035317.D
 Acq On : 19 Apr 2024 18:47
 Operator : SY/MD
 Sample : P2182-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	175323	185404	11.94%	1.577%
2	1.529	146	152	168	rVB	165537	196578	12.66%	1.672%
3	2.060	308	317	329	rBV	309854	445267	28.68%	3.788%
4	2.497	449	453	456	rBV3	570	517	0.03%	0.004%
5	2.577	475	478	479	rBV2	605	389	0.03%	0.003%
6	2.793	542	545	551	rBV3	460	519	0.03%	0.004%
7	2.844	558	561	563	rBV2	295	189	0.01%	0.002%
8	2.857	563	565	566	rVV2	282	114	0.01%	0.001%
9	2.896	569	577	590	rVV6	3039	6757	0.44%	0.057%
10	3.034	617	620	621	rBV	447	241	0.02%	0.002%
11	3.069	629	631	634	rBV2	116	70	0.00%	0.001%
12	3.085	634	636	641	rBV2	375	344	0.02%	0.003%
13	3.143	650	654	657	rBV3	339	179	0.01%	0.002%
14	3.191	665	669	672	rVB4	391	324	0.02%	0.003%
15	3.220	675	678	681	rBV3	371	193	0.01%	0.002%
16	3.278	694	696	698	rVB	169	70	0.00%	0.001%
17	3.307	700	705	714	rVB2	465	387	0.02%	0.003%
18	3.343	714	716	720	rVB	118	89	0.01%	0.001%
19	3.362	720	722	726	rBV2	282	252	0.02%	0.002%
20	3.484	756	760	761	rBV	173	118	0.01%	0.001%
21	3.494	761	763	766	rVB2	262	152	0.01%	0.001%
22	3.529	772	774	778	rBV	230	173	0.01%	0.001%
23	3.619	801	802	808	rVB	323	191	0.01%	0.002%
24	3.645	808	810	813	rBV	143	76	0.00%	0.001%
25	3.667	815	817	821	rVB3	401	240	0.02%	0.002%
26	3.786	846	854	886	rBV	124803	355228	22.88%	3.022%
27	4.246	982	997	1030	rBV	249863	645813	41.60%	5.494%
28	4.722	1142	1145	1146	rBV2	313	216	0.01%	0.002%
29	4.754	1152	1155	1158	rBV2	454	367	0.02%	0.003%
30	4.822	1173	1176	1178	rBV3	327	262	0.02%	0.002%
31	4.857	1185	1187	1189	rBV	314	109	0.01%	0.001%
32	4.899	1196	1200	1201	rBV2	380	186	0.01%	0.002%
33	4.953	1202	1217	1256	rVV2	582415	1552317	100.00%	13.205%
34	5.387	1351	1352	1354	rBV	294	128	0.01%	0.001%
35	5.461	1370	1375	1376	rBV	247	233	0.02%	0.002%
36	5.532	1386	1397	1433	rBV	431911	902978	58.17%	7.681%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035317.D
 Acq On : 19 Apr 2024 18:47
 Operator : SY/MD
 Sample : P2182-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.838	1482	1492	1506	rBV4	6727	15350	0.99%	0.131%
38	5.986	1525	1538	1568	rBV	349497	733545	47.25%	6.240%
39	6.426	1673	1675	1678	rVB2	525	243	0.02%	0.002%
40	6.445	1678	1681	1685	rBV2	447	289	0.02%	0.002%
41	6.465	1685	1687	1689	rBV2	205	98	0.01%	0.001%
42	6.513	1699	1702	1704	rBV2	616	378	0.02%	0.003%
43	6.567	1717	1719	1723	rVB	240	125	0.01%	0.001%
44	6.609	1723	1732	1733	rBV	676	646	0.04%	0.005%
45	6.696	1756	1759	1761	rVB3	292	174	0.01%	0.001%
46	6.780	1783	1785	1788	rVB2	254	123	0.01%	0.001%
47	6.799	1788	1791	1793	rBV	242	135	0.01%	0.001%
48	6.834	1797	1802	1805	rBV	287	194	0.01%	0.002%
49	6.912	1816	1826	1856	rBV	159926	319708	20.60%	2.720%
50	7.243	1914	1929	1959	rBV	636787	1141304	73.52%	9.709%
51	7.555	2017	2026	2056	rBV	111568	208896	13.46%	1.777%
52	7.857	2116	2120	2122	rBV2	383	289	0.02%	0.002%
53	7.928	2139	2142	2143	rBV	348	152	0.01%	0.001%
54	8.024	2163	2172	2225	rBV2	353925	800115	51.54%	6.806%
55	8.506	2320	2322	2324	rVB2	483	188	0.01%	0.002%
56	8.580	2343	2345	2350	rVB3	600	367	0.02%	0.003%
57	8.783	2397	2408	2442	rBV	671530	1146117	73.83%	9.750%
58	9.185	2529	2533	2534	rBV2	314	193	0.01%	0.002%
59	9.297	2566	2568	2571	rBV2	403	264	0.02%	0.002%
60	9.362	2583	2588	2589	rBV3	268	207	0.01%	0.002%
61	9.445	2610	2614	2617	rBV2	476	366	0.02%	0.003%
62	9.464	2617	2620	2624	rBV3	270	278	0.02%	0.002%
63	9.538	2635	2643	2644	rBV	310	406	0.03%	0.003%
64	9.561	2648	2650	2652	rBV2	213	74	0.00%	0.001%
65	9.725	2699	2701	2707	rVB2	383	241	0.02%	0.002%
66	9.751	2707	2709	2711	rBV2	266	177	0.01%	0.002%
67	9.831	2731	2734	2737	rBV2	339	214	0.01%	0.002%
68	9.876	2746	2748	2751	rVB	342	196	0.01%	0.002%
69	9.960	2770	2774	2776	rBV	239	184	0.01%	0.002%
70	9.985	2780	2782	2784	rVV2	400	169	0.01%	0.001%
71	9.998	2784	2786	2789	rVV	285	147	0.01%	0.001%
72	10.014	2789	2791	2792	rVB	238	83	0.01%	0.001%
73	10.059	2799	2805	2807	rBV2	304	287	0.02%	0.002%
74	10.072	2807	2809	2810	rBV	257	104	0.01%	0.001%
75	10.108	2818	2820	2821	rBV	163	71	0.00%	0.001%
76	10.149	2822	2833	2864	rVV	541371	864039	55.66%	7.350%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035317.D
 Acq On : 19 Apr 2024 18:47
 Operator : SY/MD
 Sample : P2182-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.362	2896	2899	2901	rBV	316	253	0.02%	0.002%
78	10.390	2907	2908	2911	rVB2	467	168	0.01%	0.001%
79	10.416	2912	2916	2920	rBV3	395	386	0.02%	0.003%
80	10.439	2920	2923	2925	rVB	249	141	0.01%	0.001%
81	10.452	2925	2927	2931	rBV2	290	241	0.02%	0.002%
82	10.487	2934	2938	2940	rBV2	361	348	0.02%	0.003%
83	10.564	2959	2962	2963	rBV	242	124	0.01%	0.001%
84	10.619	2977	2979	2982	rBV	304	200	0.01%	0.002%
85	10.718	3008	3010	3016	rBV2	362	279	0.02%	0.002%
86	10.863	3053	3055	3057	rBV	255	116	0.01%	0.001%
87	10.972	3087	3089	3091	rBV2	450	225	0.01%	0.002%
88	11.066	3117	3118	3120	rVB2	266	96	0.01%	0.001%
89	11.136	3134	3140	3143	rBV4	1306	1435	0.09%	0.012%
90	11.185	3143	3155	3178	rBV	651914	1042673	67.17%	8.870%
91	11.500	3243	3253	3259	rBV5	8898	16388	1.06%	0.139%
92	11.558	3261	3271	3297	rVB	714703	1147444	73.92%	9.761%
93	11.860	3363	3365	3369	rBV3	541	248	0.02%	0.002%
94	11.940	3388	3390	3393	rBV3	547	269	0.02%	0.002%
95	12.435	3541	3544	3545	rBV	457	222	0.01%	0.002%
96	12.940	3699	3701	3706	rBV2	400	287	0.02%	0.002%
97	13.111	3751	3754	3755	rBV	254	142	0.01%	0.001%
98	13.201	3777	3782	3793	rVB4	6166	9430	0.61%	0.080%
99	13.423	3847	3851	3855	rBV	414	443	0.03%	0.004%
100	13.972	4019	4022	4033	rBV3	804	1182	0.08%	0.010%




Sum of corrected areas: 11755546

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035317.D
Acq On : 19 Apr 2024 18:47
Operator : SY/MD
Sample : P2182-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

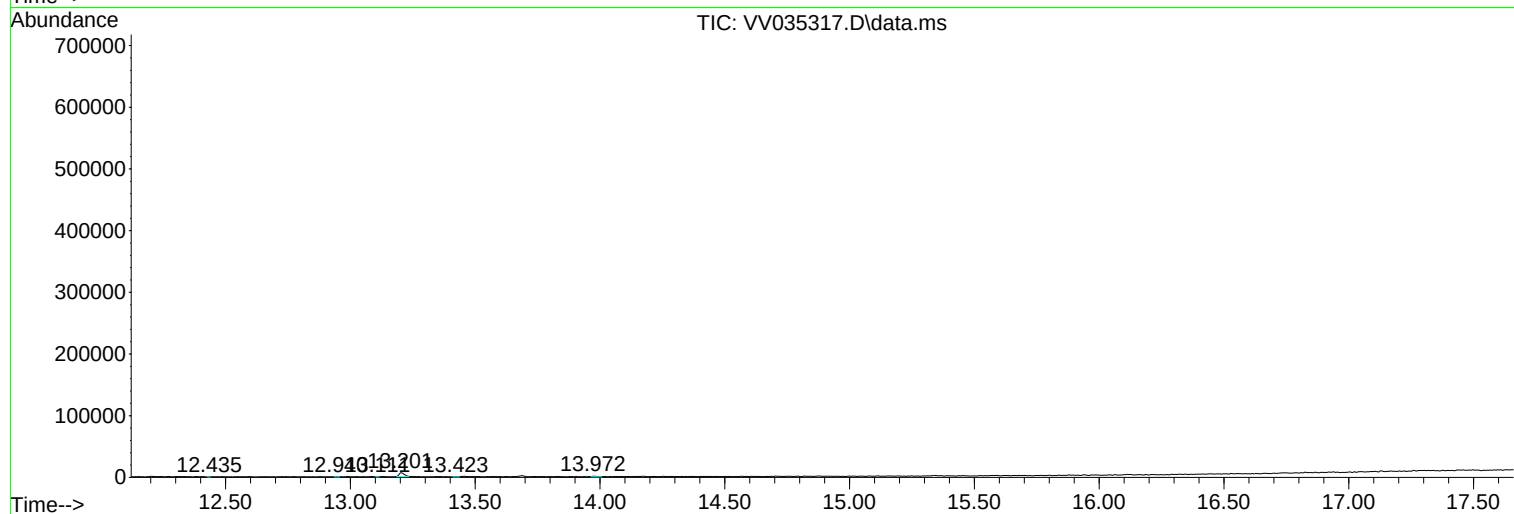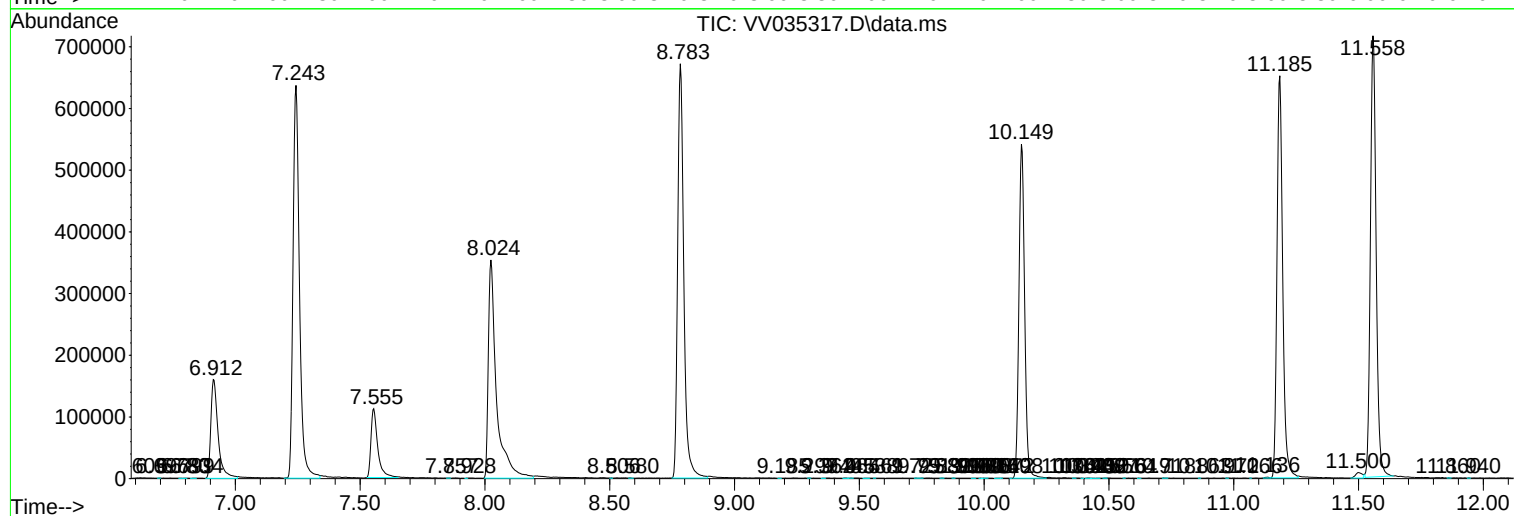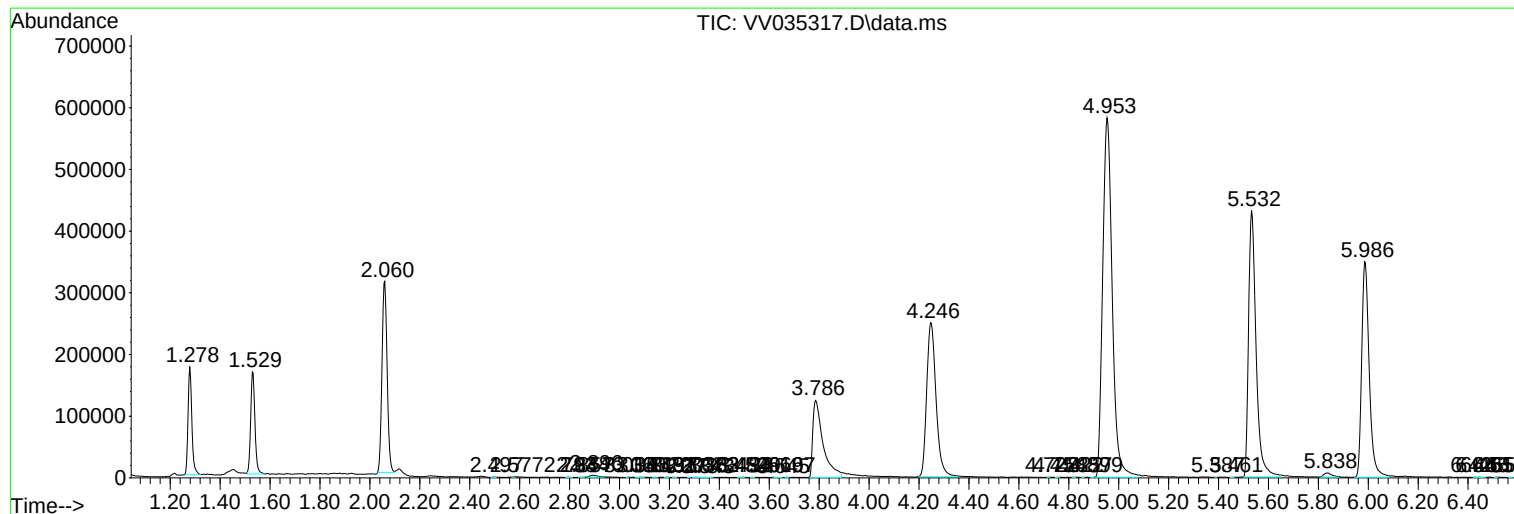

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035317.D
Acq On : 19 Apr 2024 18:47
Operator : SY/MD
Sample : P2182-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035317.D
Acq On : 19 Apr 2024 18:47
Operator : SY/MD
Sample : P2182-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------