

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035318.D
 Acq On : 19 Apr 2024 19:10
 Operator : SY/MD
 Sample : P2182-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	175225	187021	12.14%	1.605%
2	1.532	146	153	167	rVB	161370	192119	12.47%	1.649%
3	2.059	308	317	329	rBV	301878	433834	28.16%	3.723%
4	2.648	499	500	503	rBV2	339	181	0.01%	0.002%
5	2.992	604	607	608	rBV2	268	129	0.01%	0.001%
6	3.121	645	647	649	rBV	233	101	0.01%	0.001%
7	3.240	682	684	687	rBV2	249	151	0.01%	0.001%
8	3.268	691	693	696	rBV2	247	147	0.01%	0.001%
9	3.330	708	712	715	rBV2	284	219	0.01%	0.002%
10	3.410	734	737	739	rBV	195	150	0.01%	0.001%
11	3.448	747	749	751	rBV	140	60	0.00%	0.001%
12	3.522	770	772	777	rVB2	358	232	0.02%	0.002%
13	3.548	777	780	783	rBV3	449	305	0.02%	0.003%
14	3.609	793	799	800	rBV	317	227	0.01%	0.002%
15	3.670	814	818	820	rBV2	220	168	0.01%	0.001%
16	3.699	825	827	830	rVV2	229	136	0.01%	0.001%
17	3.741	838	840	843	rVB2	383	207	0.01%	0.002%
18	3.757	843	845	846	rBV2	262	100	0.01%	0.001%
19	3.786	846	854	893	rBV	124071	357012	23.18%	3.064%
20	4.249	982	998	1034	rBV	246494	640321	41.57%	5.495%
21	4.603	1106	1108	1114	rVB2	526	292	0.02%	0.003%
22	4.657	1121	1125	1129	rBV3	672	621	0.04%	0.005%
23	4.725	1144	1146	1148	rBV	378	162	0.01%	0.001%
24	4.838	1178	1181	1184	rBV2	440	265	0.02%	0.002%
25	4.870	1189	1191	1195	rBV3	249	157	0.01%	0.001%
26	4.953	1202	1217	1261	rBV2	578850	1540383	100.00%	13.220%
27	5.464	1373	1376	1377	rBV	438	191	0.01%	0.002%
28	5.532	1386	1397	1432	rBV	426389	898266	58.31%	7.709%
29	5.834	1482	1491	1509	rBV3	7066	15310	0.99%	0.131%
30	5.985	1525	1538	1574	rBV	348686	729698	47.37%	6.262%
31	6.313	1637	1640	1643	rVB3	558	280	0.02%	0.002%
32	6.374	1657	1659	1664	rVB3	737	502	0.03%	0.004%
33	6.403	1664	1668	1671	rBV	380	389	0.03%	0.003%
34	6.751	1774	1776	1780	rBV3	374	213	0.01%	0.002%
35	6.815	1793	1796	1800	rBV2	209	140	0.01%	0.001%
36	6.870	1809	1813	1815	rBV2	270	229	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
 Data File : VV035318.D
 Acq On : 19 Apr 2024 19:10
 Operator : SY/MD
 Sample : P2182-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R82

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.911	1816	1826	1853	rBV	158179	311094	20.20%	2.670%
38	7.156	1898	1902	1909	rBV6	674	1102	0.07%	0.009%
39	7.243	1917	1929	1958	rBV	623716	1125436	73.06%	9.658%
40	7.554	2016	2026	2059	rBV	108828	213426	13.86%	1.832%
41	7.850	2113	2118	2120	rBV3	474	392	0.03%	0.003%
42	7.950	2147	2149	2151	rVB	231	53	0.00%	0.000%
43	7.992	2159	2162	2163	rBV	283	141	0.01%	0.001%
44	8.024	2163	2172	2216	rBV2	346373	774610	50.29%	6.648%
45	8.580	2343	2345	2349	rBV2	621	454	0.03%	0.004%
46	8.615	2354	2356	2358	rBV2	450	208	0.01%	0.002%
47	8.783	2397	2408	2440	rBV	686854	1145096	74.34%	9.827%
48	9.130	2514	2516	2519	rBV4	350	179	0.01%	0.002%
49	9.262	2555	2557	2561	rVB2	461	267	0.02%	0.002%
50	9.281	2561	2563	2564	rBV	218	50	0.00%	0.000%
51	9.307	2566	2571	2574	rVV3	357	387	0.03%	0.003%
52	9.332	2577	2579	2582	rVB2	292	164	0.01%	0.001%
53	9.365	2583	2589	2592	rBV3	481	435	0.03%	0.004%
54	9.477	2621	2624	2630	rVB3	573	432	0.03%	0.004%
55	9.522	2636	2638	2645	rVB2	656	636	0.04%	0.005%
56	9.590	2658	2659	2664	rVB3	224	144	0.01%	0.001%
57	9.812	2726	2728	2729	rBV	346	107	0.01%	0.001%
58	9.841	2735	2737	2740	rBV2	250	98	0.01%	0.001%
59	9.873	2745	2747	2751	rBV2	291	173	0.01%	0.001%
60	9.911	2757	2759	2760	rBV	177	47	0.00%	0.000%
61	9.976	2775	2779	2786	rBV4	390	449	0.03%	0.004%
62	10.050	2798	2802	2804	rBV2	464	316	0.02%	0.003%
63	10.149	2822	2833	2856	rBV	544291	850774	55.23%	7.301%
64	10.374	2900	2903	2906	rBV3	361	228	0.01%	0.002%
65	10.394	2906	2909	2911	rBV2	339	198	0.01%	0.002%
66	10.496	2939	2941	2944	rBV2	305	191	0.01%	0.002%
67	10.834	3043	3046	3048	rBV3	217	126	0.01%	0.001%
68	10.879	3057	3060	3063	rVB	283	136	0.01%	0.001%
69	10.898	3063	3066	3068	rBV2	321	190	0.01%	0.002%
70	11.082	3121	3123	3125	rBV2	298	175	0.01%	0.002%
71	11.185	3144	3155	3183	rBV	650409	1038064	67.39%	8.909%
72	11.493	3242	3251	3260	rBV3	18303	36974	2.40%	0.317%
73	11.557	3261	3271	3294	rVB	714217	1140112	74.01%	9.784%
74	11.982	3399	3403	3408	rBV4	499	517	0.03%	0.004%
75	12.082	3431	3434	3435	rBV4	441	265	0.02%	0.002%
76	12.892	3684	3686	3688	rBV2	560	288	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035318.D
Acq On : 19 Apr 2024 19:10
Operator : SY/MD
Sample : P2182-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R82

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Title : VOC Analysis

77	13.210	3777	3785	3792	rBV8	4762	7627	0.50%	0.065%
78	13.680	3928	3931	3932	rBV2	947	612	0.04%	0.005%


Sum of corrected areas: 11652291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035318.D
Acq On : 19 Apr 2024 19:10
Operator : SY/MD
Sample : P2182-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

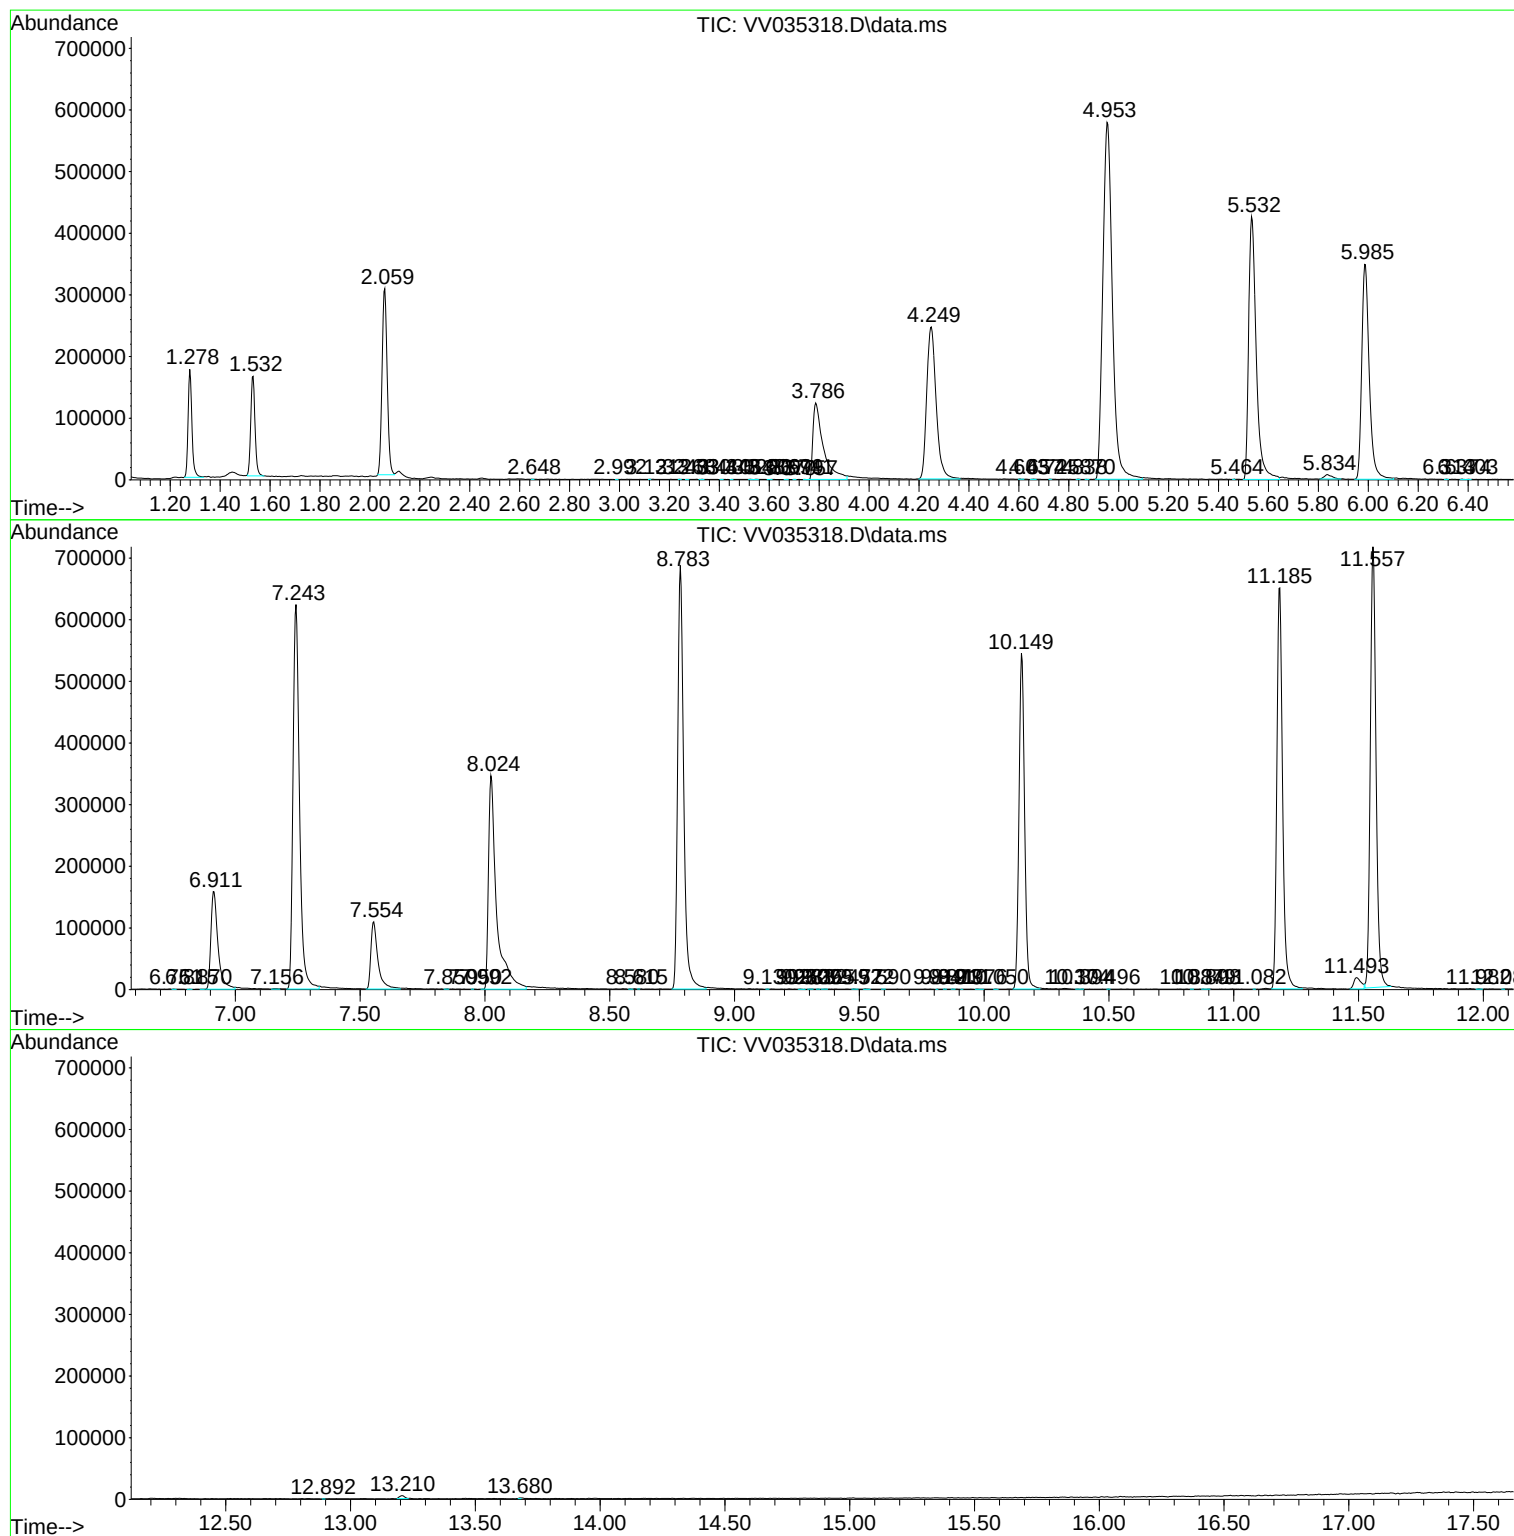

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035318.D
Acq On : 19 Apr 2024 19:10
Operator : SY/MD
Sample : P2182-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041924\
Data File : VV035318.D
Acq On : 19 Apr 2024 19:10
Operator : SY/MD
Sample : P2182-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R82

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------