




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025649.D
 Acq On : 20 Apr 2022 16:23
 Operator : SY/MD
 Sample : N2492-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:44:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

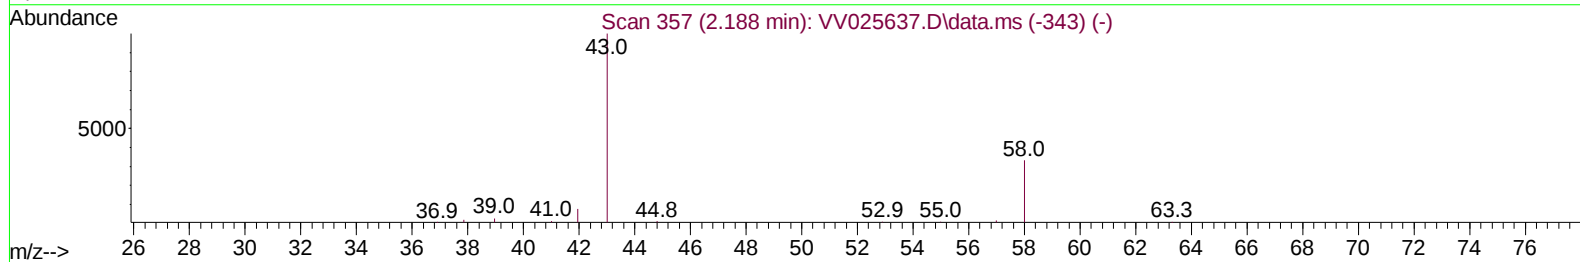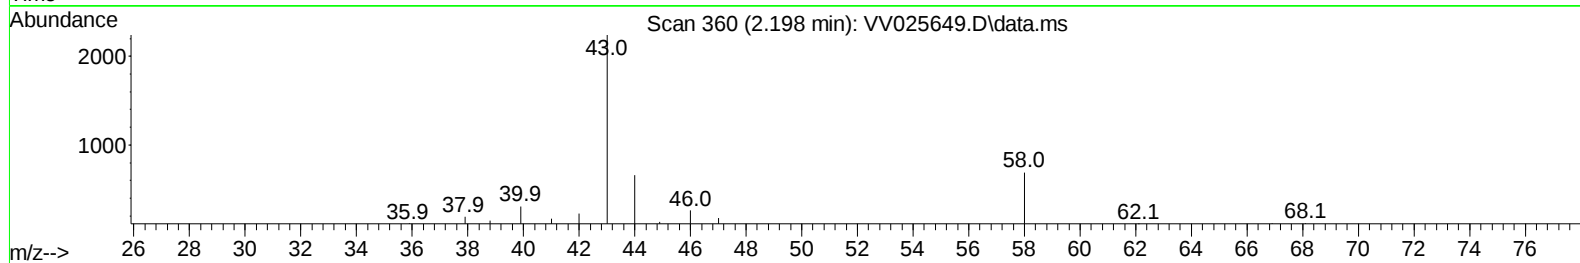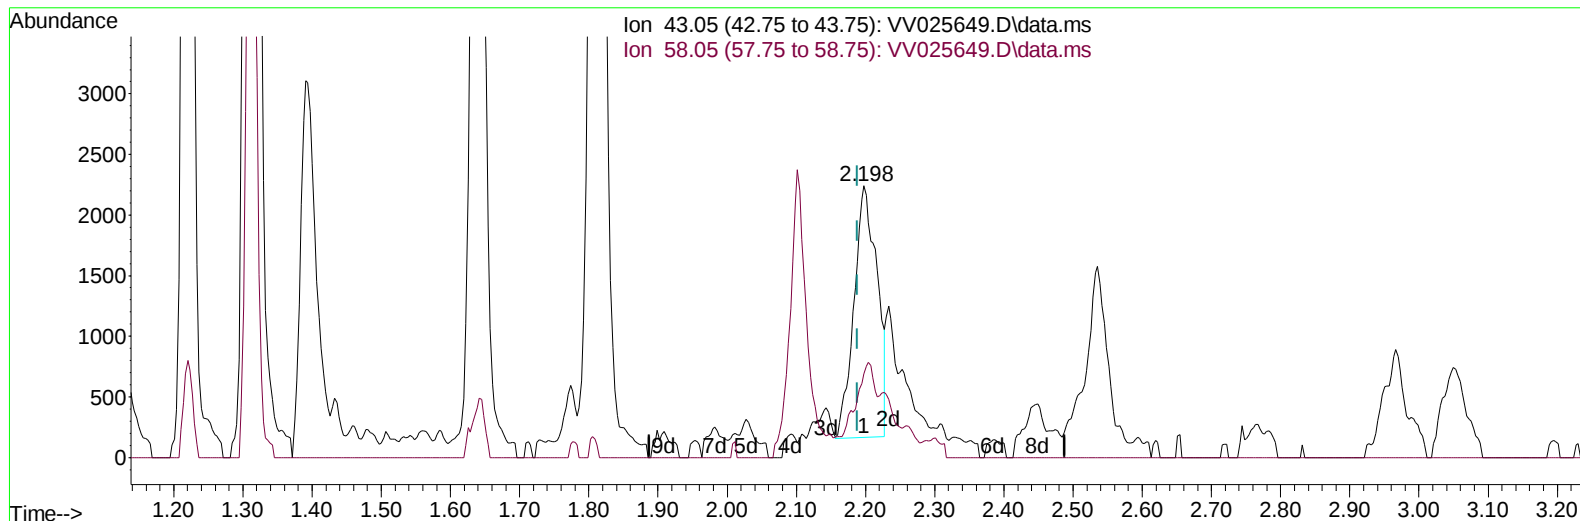

TIC: VV025649.D\data.ms

(13) Acetone (T)

2.198min (+ 0.010) 5.52 ug/L

response 4809

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	22.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025649.D
Acq On : 20 Apr 2022 16:23
Operator : SY/MD
Sample : N2492-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

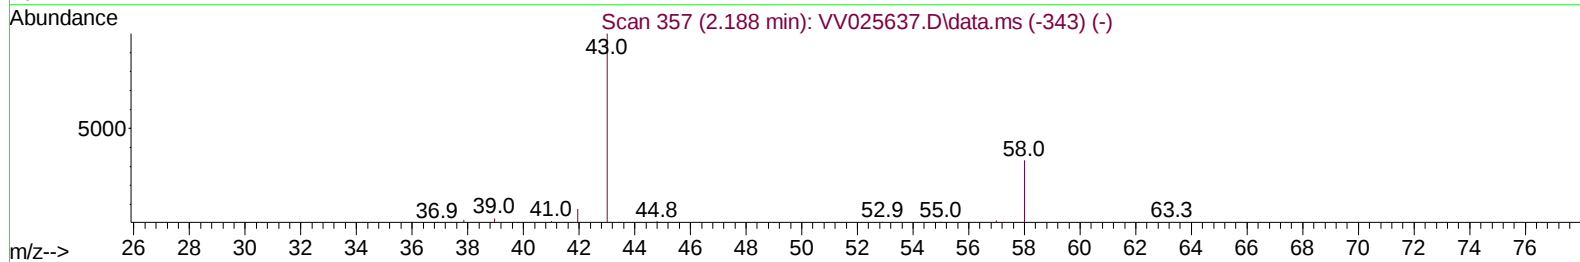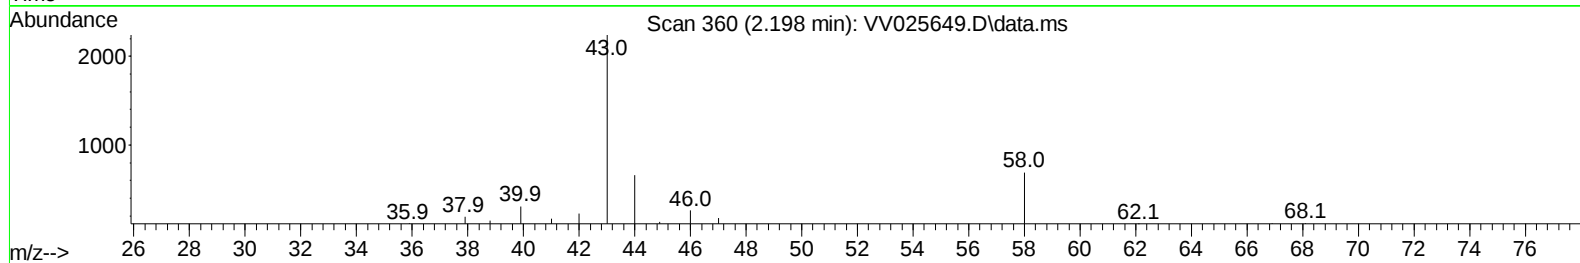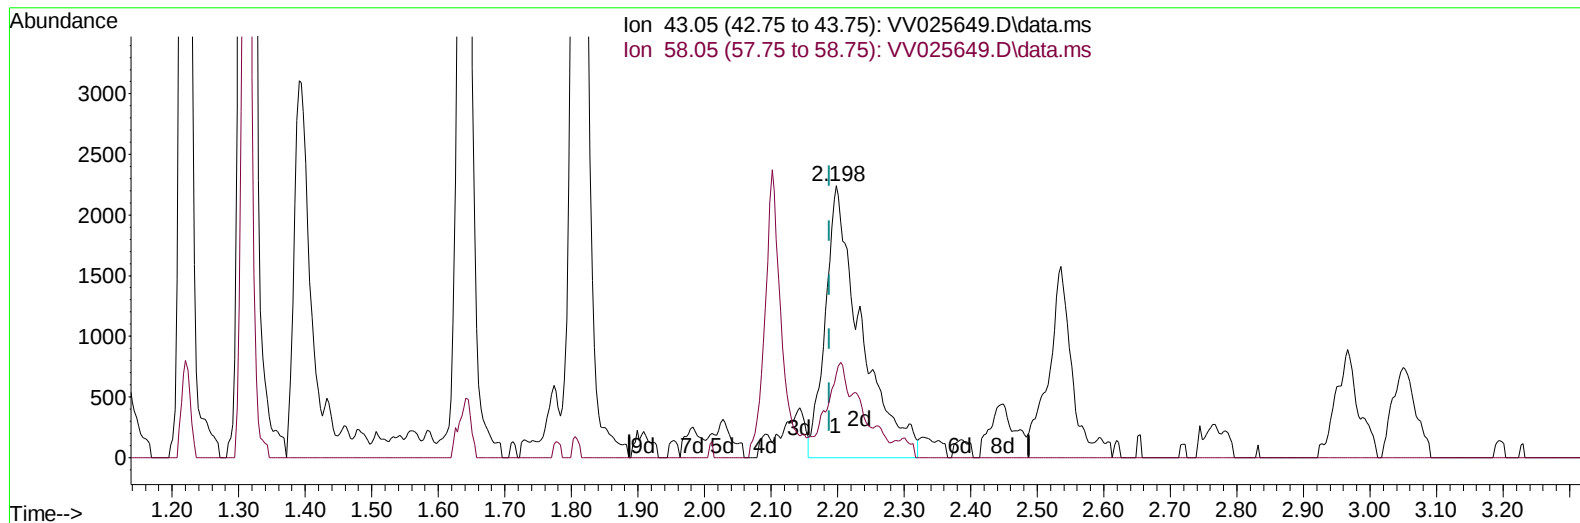

TIC: VV025649.D\data.ms

(13) Acetone (T)

2.198min (+ 0.010) 9.56 ug/L m

response 8323

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	12.94
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025649.D
 Acq On : 20 Apr 2022 16:23
 Operator : SY/MD
 Sample : N2492-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T8

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:44:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		113471	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		118847	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		52392	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.310	65		43629	4.136	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	82.800%		
7) Chloroethane-d5	1.571	69		44157	3.934	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	78.600%		
11) 1,1-Dichloroethene-d2	2.114	63		67833	3.210	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	64.200%		
20) 2-Butanone-d5	3.905	46		82946	64.638	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery =	129.280%		
24) Chloroform-d	4.352	84		82444	5.172	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	103.400%		
26) 1,2-Dichloroethane-d4	5.037	65		41021	5.972	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	119.400%		
32) Benzene-d6	5.053	84		157624	4.584	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	91.600%		
36) 1,2-Dichloropropane-d6	6.072	67		51268	5.346	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	107.000%		
41) Toluene-d8	7.317	98		128260	4.019	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	80.400%		
43) trans-1,3-Dichloroprop...	7.625	79		14037	4.355	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	87.000%		
46) 2-Hexanone-d5	8.088	63		58125	51.379	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	102.760%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84		32789	5.412	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	108.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152		44320	5.045	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	101.000%		
Target Compounds							
						Qvalue	
13) Acetone	2.198	43		8323m	9.556	ug/L	
30) Cyclohexane	4.677	56		1014	0.080	ug/L #	94
33) Benzene	5.111	78		7807	0.222	ug/L	100
34) Trichloroethene	5.928	95		2356	0.253	ug/L	91
35) Methylcyclohexane	6.127	83		2051	0.138	ug/L #	89
42) Toluene	7.397	91		15298	0.401	ug/L	93
47) Tetrachloroethene	7.976	164		156295	21.417	ug/L	97
52) Ethylbenzene	9.021	91		7064	0.173	ug/L	95
53) m,p-Xylene	9.149	106		2530	0.163	ug/L	78
54) o-Xylene	9.554	106		1080	0.072	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025649.D
Acq On : 20 Apr 2022 16:23
Operator : SY/MD
Sample : N2492-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T8

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

