




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025651.D
 Acq On : 20 Apr 2022 17:10
 Operator : SY/MD
 Sample : N2492-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

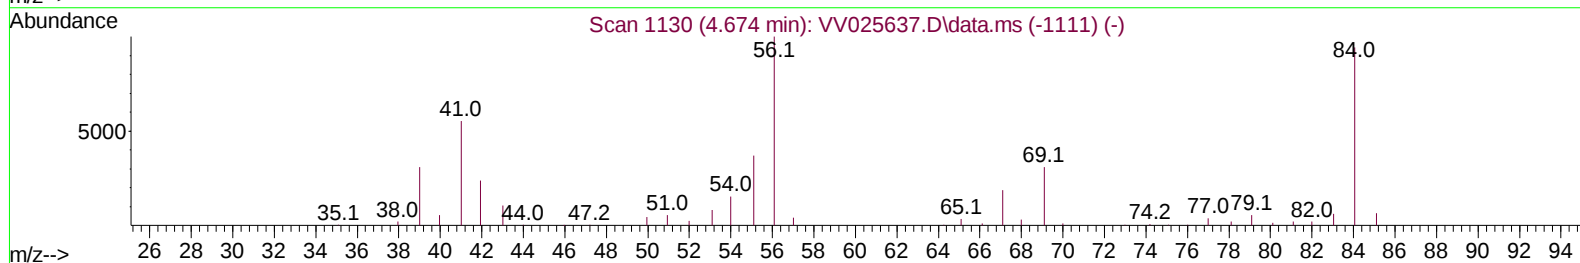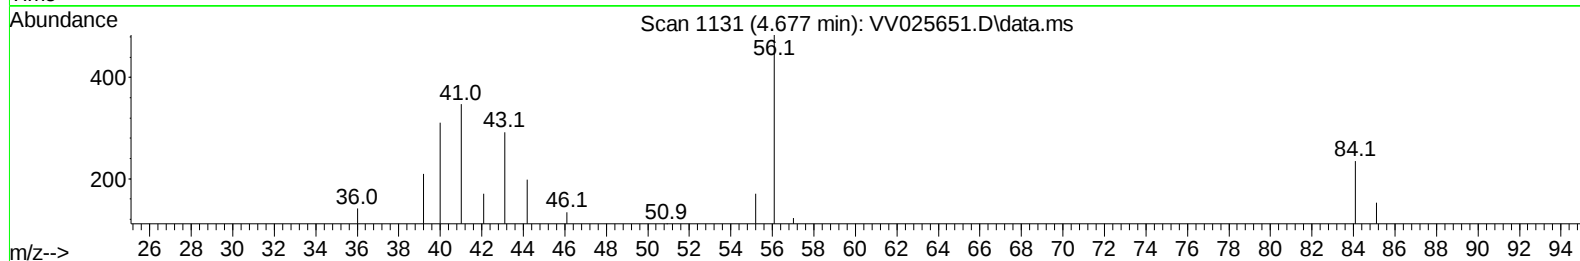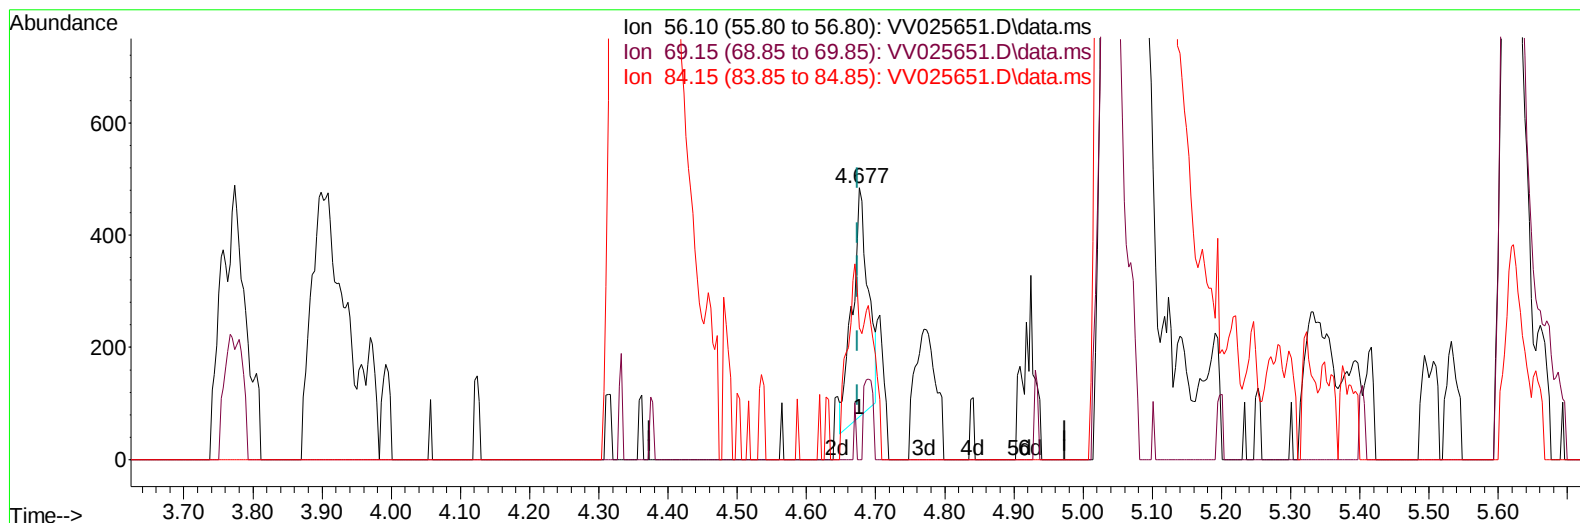

TIC: VV025651.D\data.ms

(30) Cyclohexane (T)

4.677min (+ 0.003) 0.05 ug/L

response 652

Ion	Exp%	Act%
56.10	100.00	100.00
69.15	32.60	2.91#
84.15	98.30	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025651.D
Acq On : 20 Apr 2022 17:10
Operator : SY/MD
Sample : N2492-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

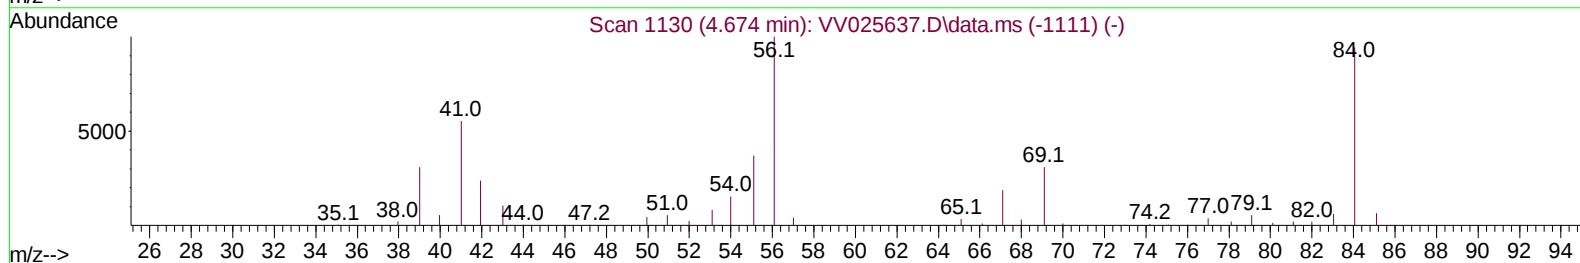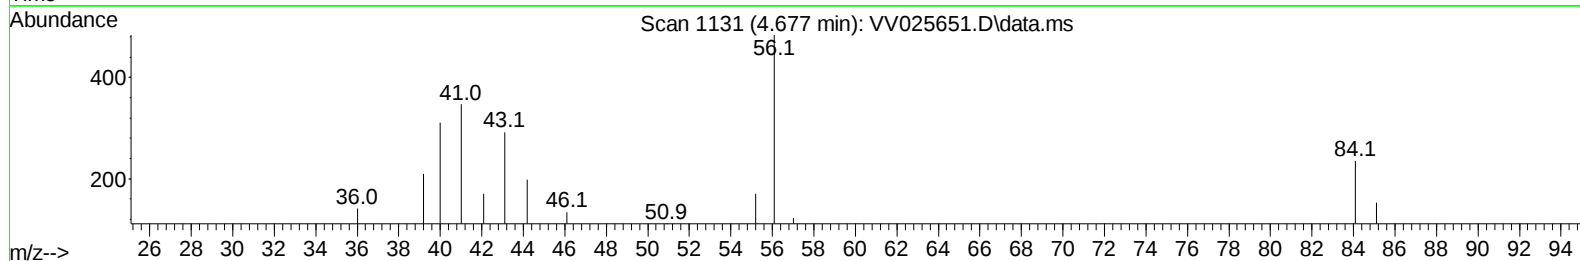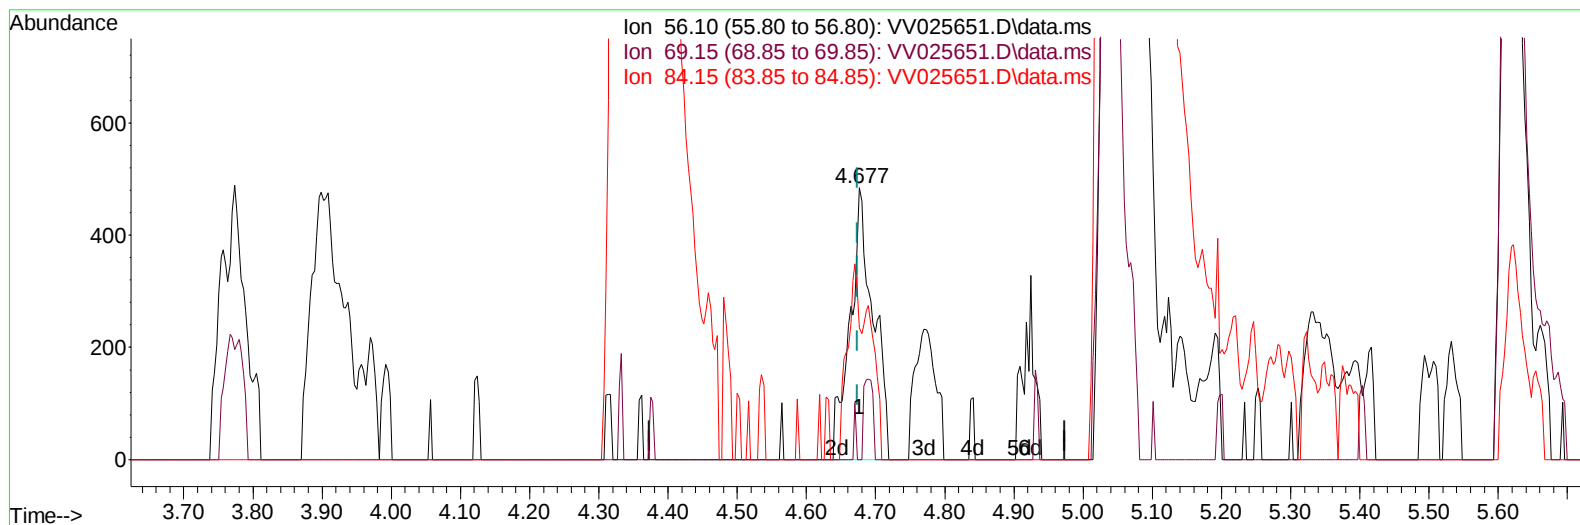

TIC: VV025651.D\data.ms

(30) Cyclohexane (T)

4.677min (+ 0.003) 0.09 ug/L m

response 1123

Ion	Exp%	Act%
56.10	100.00	100.00
69.15	32.60	1.69#
84.15	98.30	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025651.D
 Acq On : 20 Apr 2022 17:10
 Operator : SY/MD
 Sample : N2492-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	125529	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	122437	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56389	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	44656	3.826	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.600%	
7) Chloroethane-d5	1.574	69	45450	3.661	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	73.200%	
11) 1,1-Dichloroethene-d2	2.114	63	70330	3.008	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	60.200%	
20) 2-Butanone-d5	3.902	46	84667	59.641	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	119.280%	
24) Chloroform-d	4.355	84	86944	4.930	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.037	65	41887	5.512	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	110.200%	
32) Benzene-d6	5.053	84	165425	4.670	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.400%	
36) 1,2-Dichloropropane-d6	6.072	67	52759	5.340	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	106.800%	
41) Toluene-d8	7.317	98	137345	4.178	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	83.600%	
43) trans-1,3-Dichloroprop...	7.625	79	16049	4.833	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	96.600%	
46) 2-Hexanone-d5	8.088	63	68202	58.519	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	117.040%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	32804	5.256	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	46296	4.897	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	98.000%	
Target Compounds						
						Qvalue
22) cis-1,2-Dichloroethene	3.924	96	1927	0.201	ug/L	90
30) Cyclohexane	4.677	56	1123m	0.086	ug/L	
33) Benzene	5.108	78	4132	0.114	ug/L	100
34) Trichloroethene	5.918	95	34577	3.601	ug/L	97
35) Methylcyclohexane	6.137	83	2073	0.135	ug/L #	84
42) Toluene	7.397	91	11905	0.303	ug/L	99
47) Tetrachloroethene	7.982	164	8795512	1169.901	ug/L	93
52) Ethylbenzene	9.017	91	6964	0.166	ug/L	92
53) m,p-Xylene	9.146	106	1736	0.109	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025651.D
Acq On : 20 Apr 2022 17:10
Operator : SY/MD
Sample : N2492-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:44:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

