




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025654.D
 Acq On : 20 Apr 2022 18:20
 Operator : SY/MD
 Sample : N2492-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

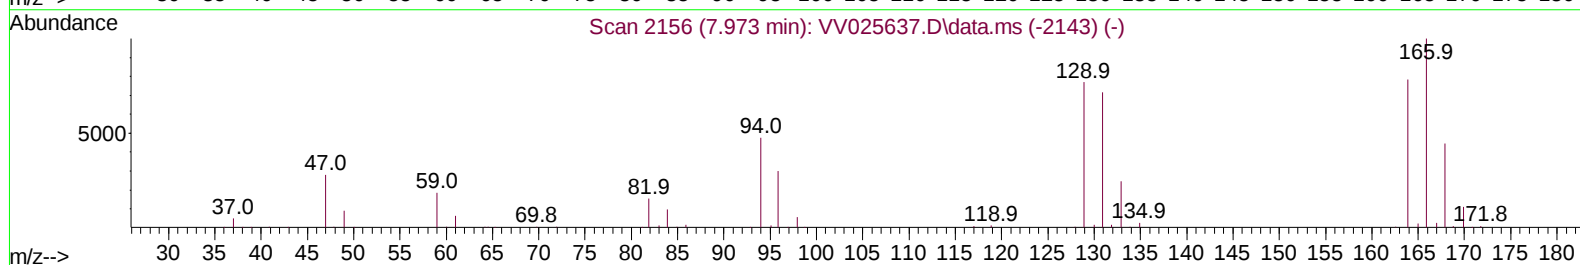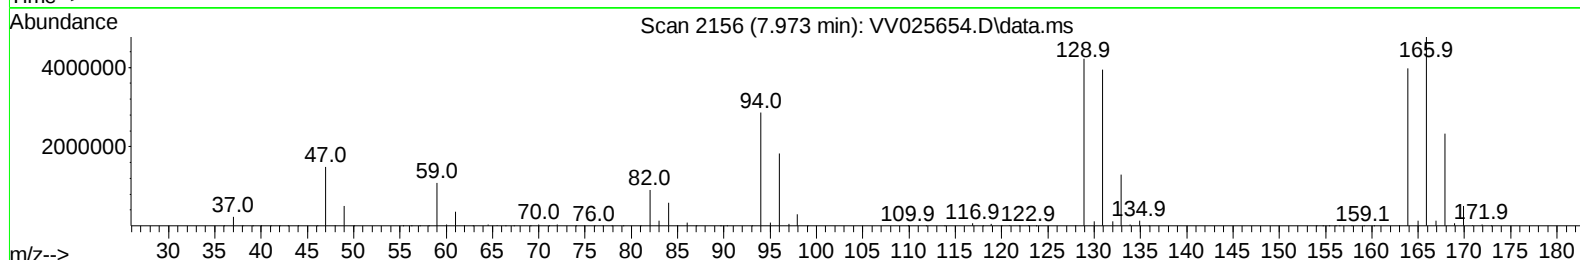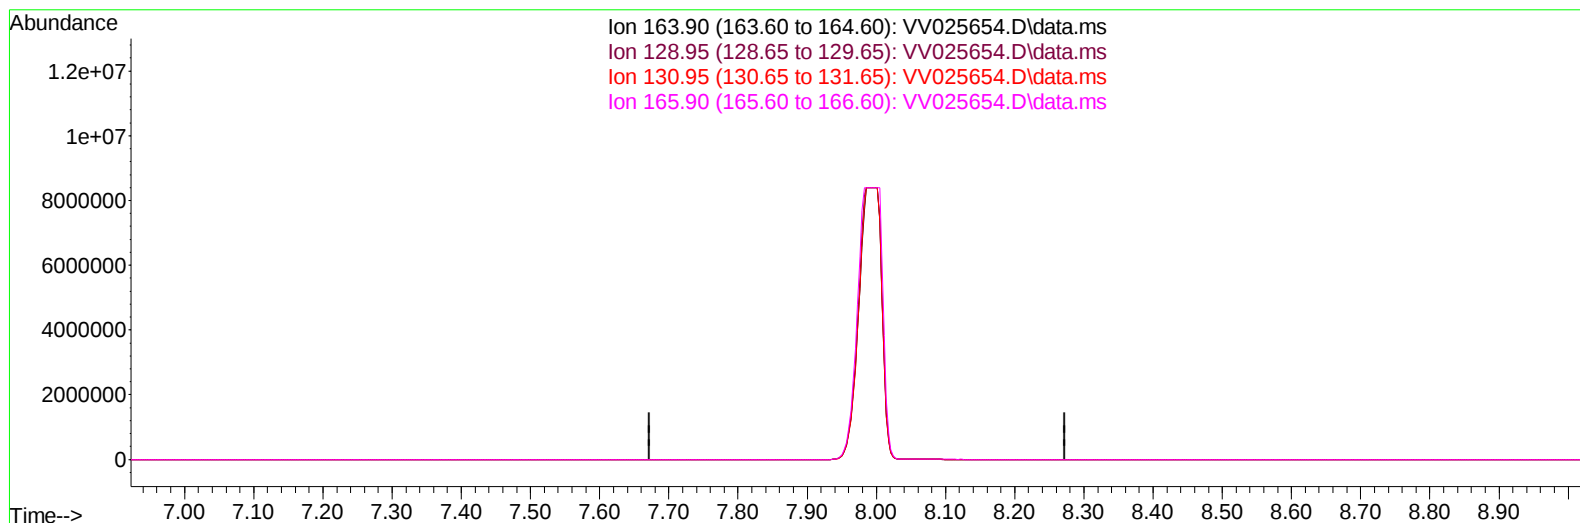

TIC: VV025654.D\data.ms

(47) Tetrachloroethene (T)

7.973min (-7.973) 0.00 ug/L

response 0

Ion	Exp%	Act%
163.90	100.00	0.00
128.95	95.50	0.00#
130.95	94.90	0.00#
165.90	131.00	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025654.D
 Acq On : 20 Apr 2022 18:20
 Operator : SY/MD
 Sample : N2492-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

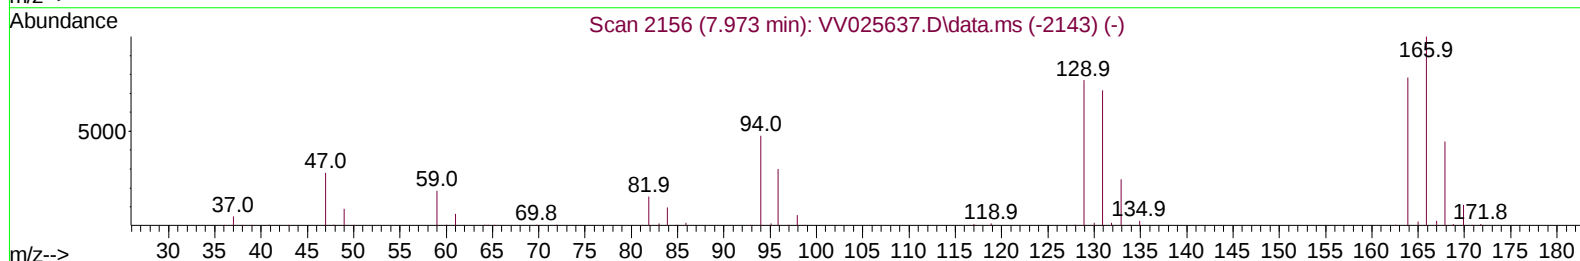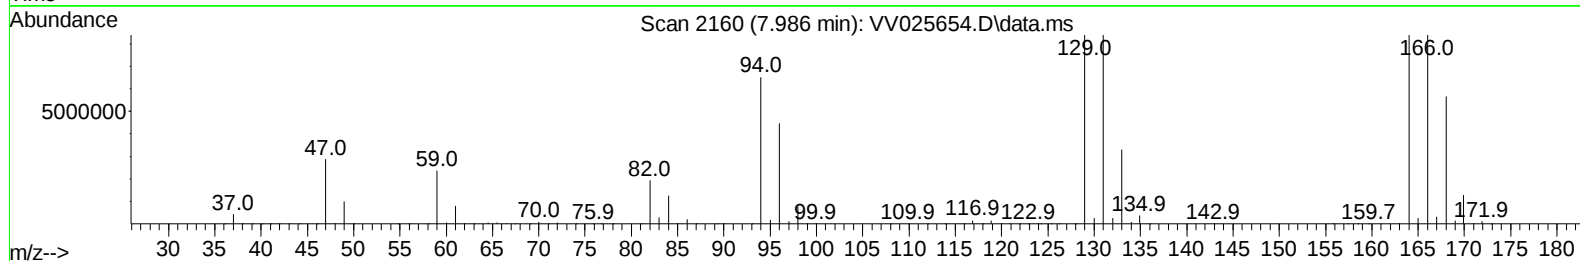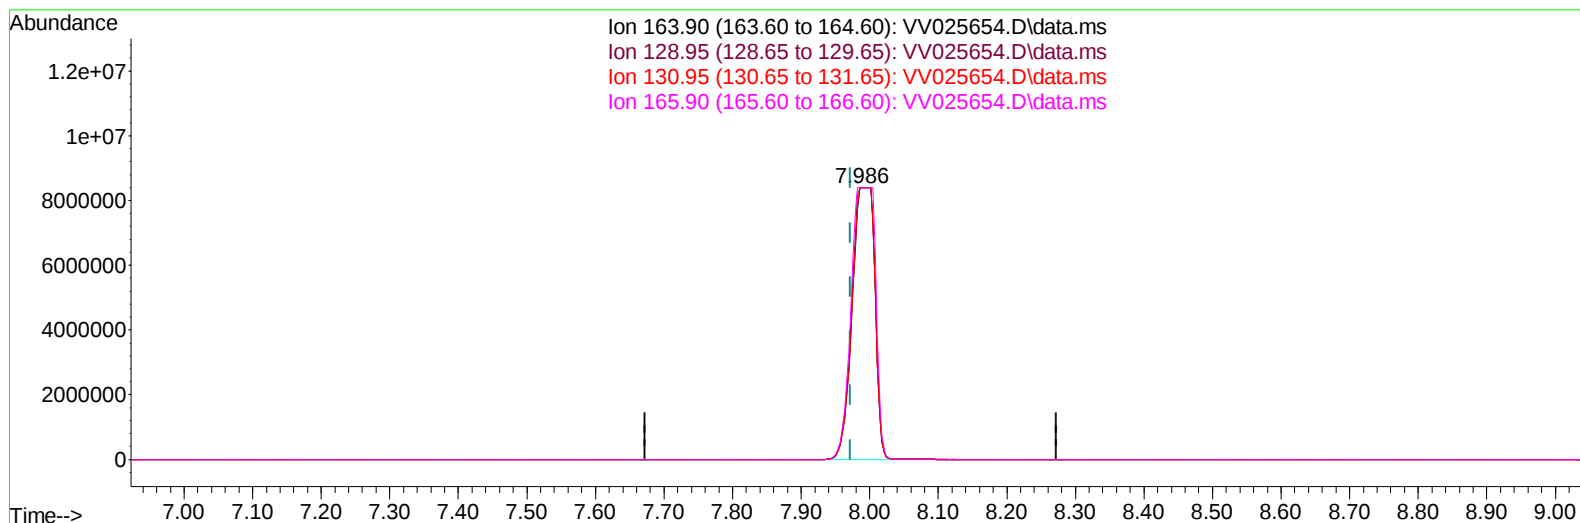

TIC: VV025654.D\data.ms

(47) Tetrachloroethene (T)

7.986min (+ 0.013) 2385.28 ug/L m

response 19221875

Ion	Exp%	Act%
163.90	100.00	100.00
128.95	95.50	100.00
130.95	94.90	100.00
165.90	131.00	100.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025654.D
 Acq On : 20 Apr 2022 18:20
 Operator : SY/MD
 Sample : N2492-11
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W3

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:45:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		133400	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		131237	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		57884	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.311	65		51781	4.175	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.600%	
7) Chloroethane-d5	1.574	69		53647	4.066	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.400%	
11) 1,1-Dichloroethene-d2	2.114	63		84226	3.390	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%	
20) 2-Butanone-d5	3.896	46		94623	62.722	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.440%	
24) Chloroform-d	4.355	84		98226	5.241	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.800%	
26) 1,2-Dichloroethane-d4	5.034	65		47915	5.934	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	118.600%	
32) Benzene-d6	5.053	84		196248	5.168	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%	
36) 1,2-Dichloropropane-d6	6.072	67		60485	5.712	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.200%	
41) Toluene-d8	7.317	98		165299	4.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%	
43) trans-1,3-Dichloroprop...	7.625	79		17729	4.981	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.600%	
46) 2-Hexanone-d5	8.088	63		77402	61.959	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.920%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		36433	5.446	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152		54696	5.636	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.800%	
Target Compounds							Qvalue
12) 1,1-Dichloroethene	2.124	96		2332	0.202	ug/L	# 1
22) cis-1,2-Dichloroethene	3.918	96		16808	1.647	ug/L	97
33) Benzene	5.114	78		4164	0.107	ug/L	100
34) Trichloroethene	5.915	95		139899	13.591	ug/L	99
47) Tetrachloroethene	7.986	164		19221875m	2385.284	ug/L	
52) Ethylbenzene	9.021	91		2685	0.060	ug/L	88
53) m,p-Xylene	9.146	106		970	0.057	ug/L	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025654.D
Acq On : 20 Apr 2022 18:20
Operator : SY/MD
Sample : N2492-11
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W3

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

