




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025656.D
 Acq On : 20 Apr 2022 19:07
 Operator : SY/MD
 Sample : N2492-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

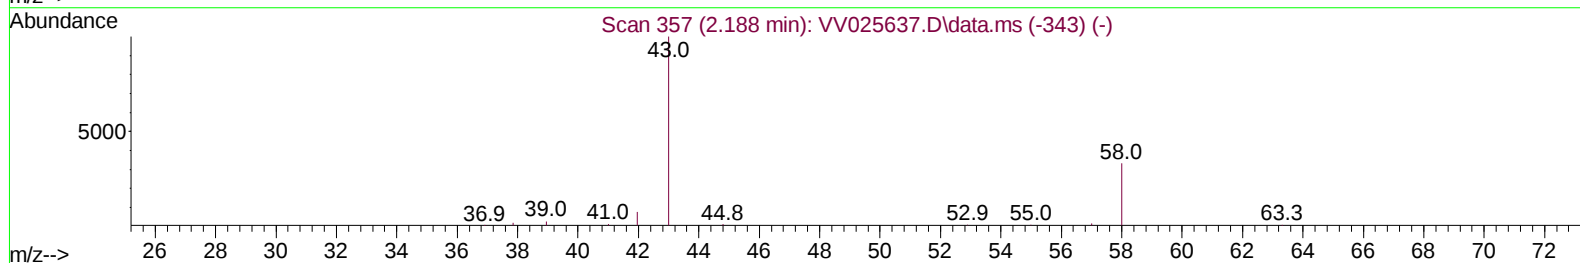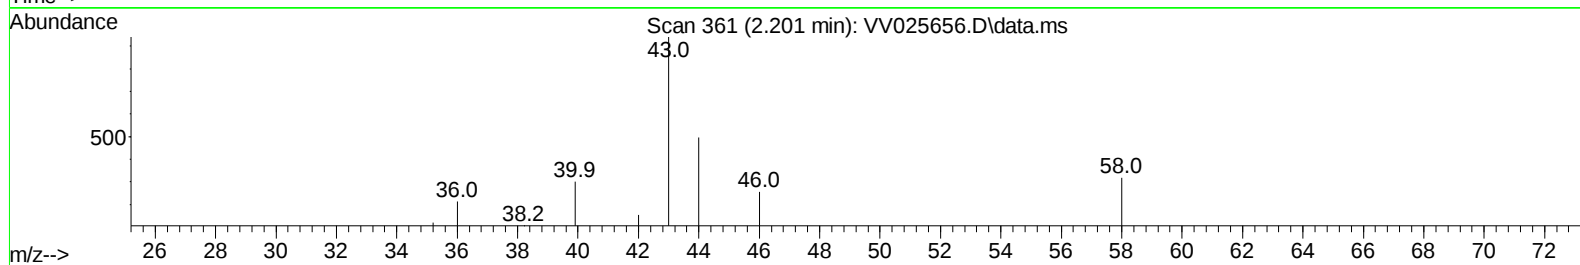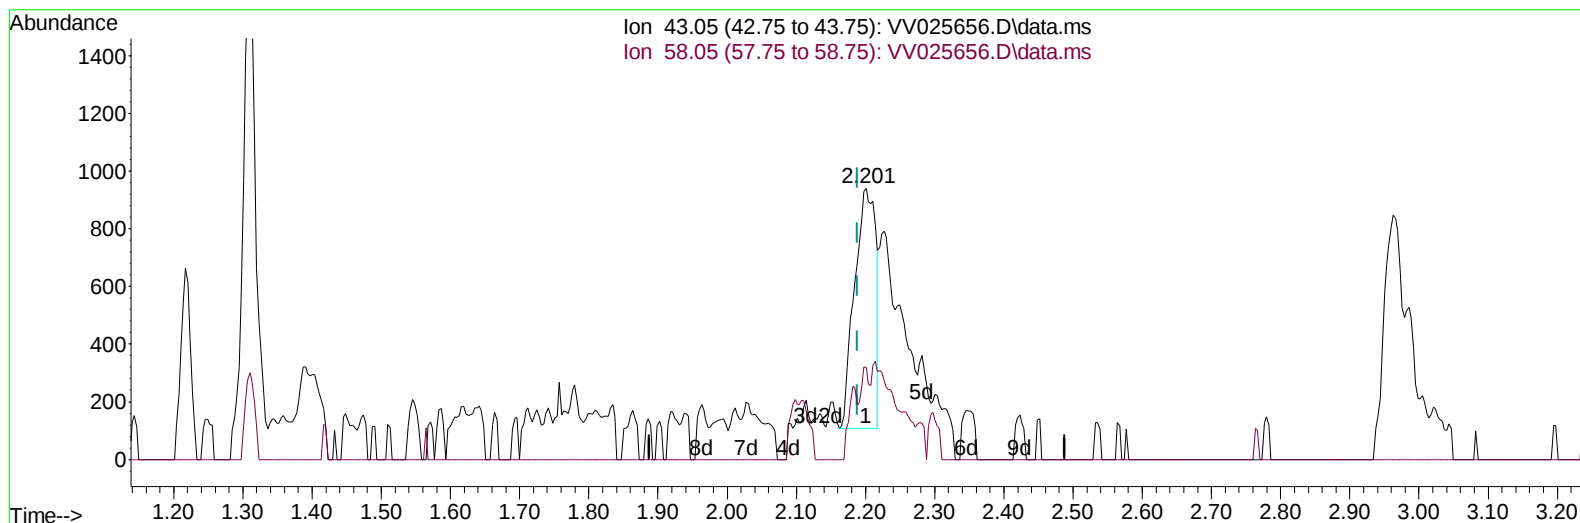

TIC: VV025656.D\data.ms

(13) Acetone (T)

2.201min (+ 0.013) 1.87 ug/L

response 1748

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	15.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025656.D
 Acq On : 20 Apr 2022 19:07
 Operator : SY/MD
 Sample : N2492-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

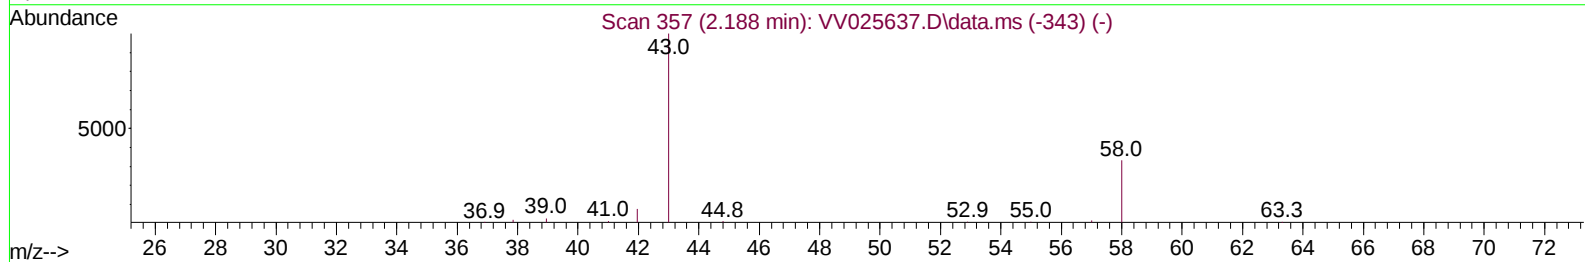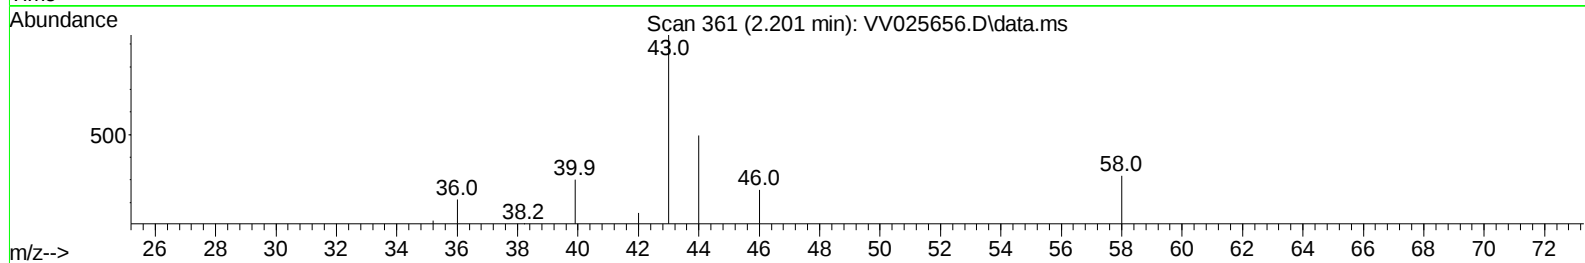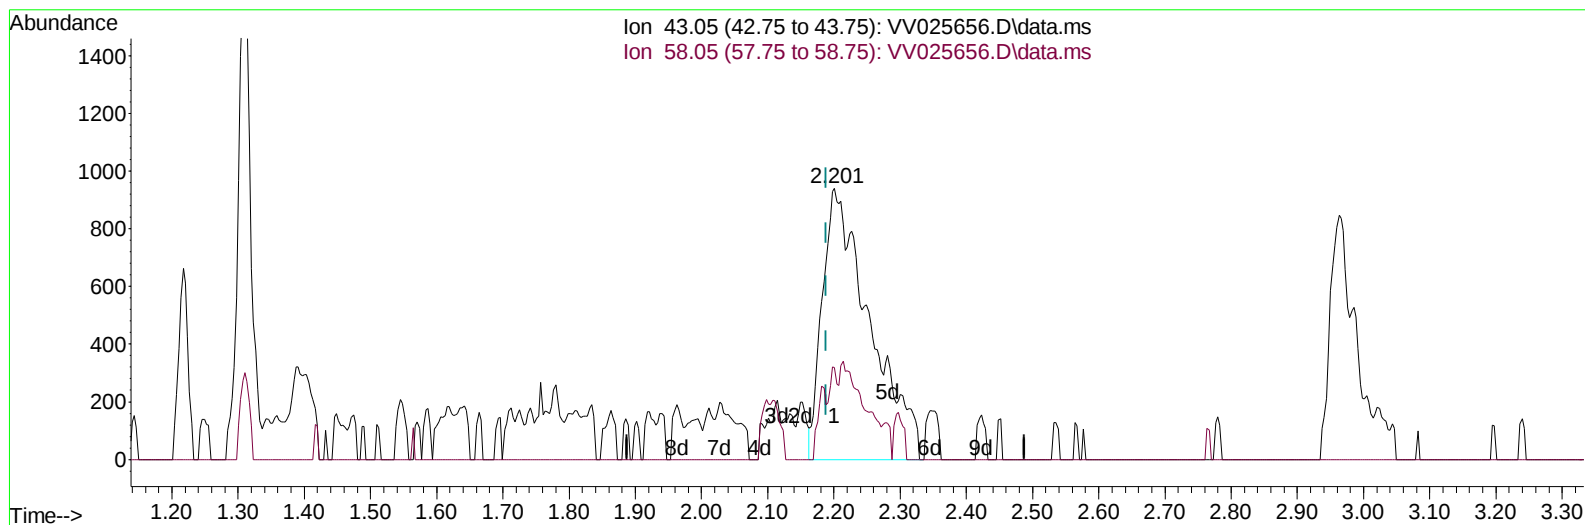

TIC: VV025656.D\data.ms

(13) Acetone (T)

2.201min (+ 0.013) 4.96 ug/L m

response 4628

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	5.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025656.D
 Acq On : 20 Apr 2022 19:07
 Operator : SY/MD
 Sample : N2492-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z6

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/21/2022
 Supervised By :Semsettin Yesilyurt 04/22/2022

Quant Time: Apr 21 06:45:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 21 06:38:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121502	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125450	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52754	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	47242	4.182	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	83.600%	
7) Chloroethane-d5	1.571	69	47188	3.927	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.111	63	76428	3.377	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	67.600%	
20) 2-Butanone-d5	3.911	46	76045	55.343	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	110.680%	
24) Chloroform-d	4.352	84	88465	5.183	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	5.037	65	42412	5.766	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	115.400%	
32) Benzene-d6	5.053	84	168384	4.639	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	92.800%	
36) 1,2-Dichloropropane-d6	6.072	67	52875	5.223	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	104.400%	
41) Toluene-d8	7.316	98	138599	4.115	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	82.200%	
43) trans-1,3-Dichloroprop...	7.625	79	15368	4.517	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.091	63	58075	48.633	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	97.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31753	4.965	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48774	5.514	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	110.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	4628m	4.962	ug/L	
16) Methylene chloride	2.513	84	4013	0.393	ug/L	90
25) Chloroform	4.381	83	21448	1.359	ug/L	90
38) Bromodichloromethane	6.519	83	2946	0.277	ug/L #	90
47) Tetrachloroethene	7.979	164	10692	1.388	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025656.D
Acq On : 20 Apr 2022 19:07
Operator : SY/MD
Sample : N2492-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 06:45:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 21 06:38:14 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/21/2022
Supervised By :Semsettin Yesilyurt 04/22/2022

