

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW042022\  
 Data File : VW025639.D  
 Acq On : 20 Apr 2022 10:53  
 Operator : SY/MD  
 Sample : N2384-21  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VHBLK001

Quant Time: Apr 21 06:42:06 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Apr 21 06:38:14 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------|----------|
| -----                         |        |       |          |          |       |          |
| Internal Standards            |        |       |          |          |       |          |
| 1) 1,4-Difluorobenzene        | 5.613  | 114   | 173772   | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.850  | 117   | 178020   | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.246 | 152   | 79717    | 5.000    | ug/L  | 0.00     |
|                               |        |       |          |          |       |          |
| System Monitoring Compounds   |        |       |          |          |       |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65    | 62999    | 3.899    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 78.000%  |
| 7) Chloroethane-d5            | 1.568  | 69    | 61969    | 3.606    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 72.200%  |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63    | 104212   | 3.220    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 64.400%  |
| 20) 2-Butanone-d5             | 3.908  | 46    | 85981    | 43.752   | ug/L  | 0.02     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 87.500%  |
| 24) Chloroform-d              | 4.346  | 84    | 110771   | 4.537    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 90.800%  |
| 26) 1,2-Dichloroethane-d4     | 5.031  | 65    | 51758    | 4.920    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 98.400%  |
| 32) Benzene-d6                | 5.047  | 84    | 213346   | 4.142    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 82.800%  |
| 36) 1,2-Dichloropropane-d6    | 6.066  | 67    | 65516    | 4.561    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 91.200%  |
| 41) Toluene-d8                | 7.313  | 98    | 179465   | 3.755    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 75.000%  |
| 43) trans-1,3-Dichloroprop... | 7.622  | 79    | 19386    | 4.015    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 80.400%  |
| 46) 2-Hexanone-d5             | 8.088  | 63    | 69248    | 40.865   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 81.720%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214 | 84    | 37952    | 4.182    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 83.600%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152   | 61359    | 4.591    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 91.800%  |
|                               |        |       |          |          |       |          |
| Target Compounds              |        |       |          |          |       | Qvalue   |
| 16) Methylene chloride        | 2.507  | 84    | 6378     | 0.436    | ug/L  | 94       |
| -----                         |        |       |          |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV042022\  
Data File : VV025639.D  
Acq On : 20 Apr 2022 10:53  
Operator : SY/MD  
Sample : N2384-21  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VHBLK001


Quant Time: Apr 21 06:42:06 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Apr 21 06:38:14 2022  
Response via : Initial Calibration

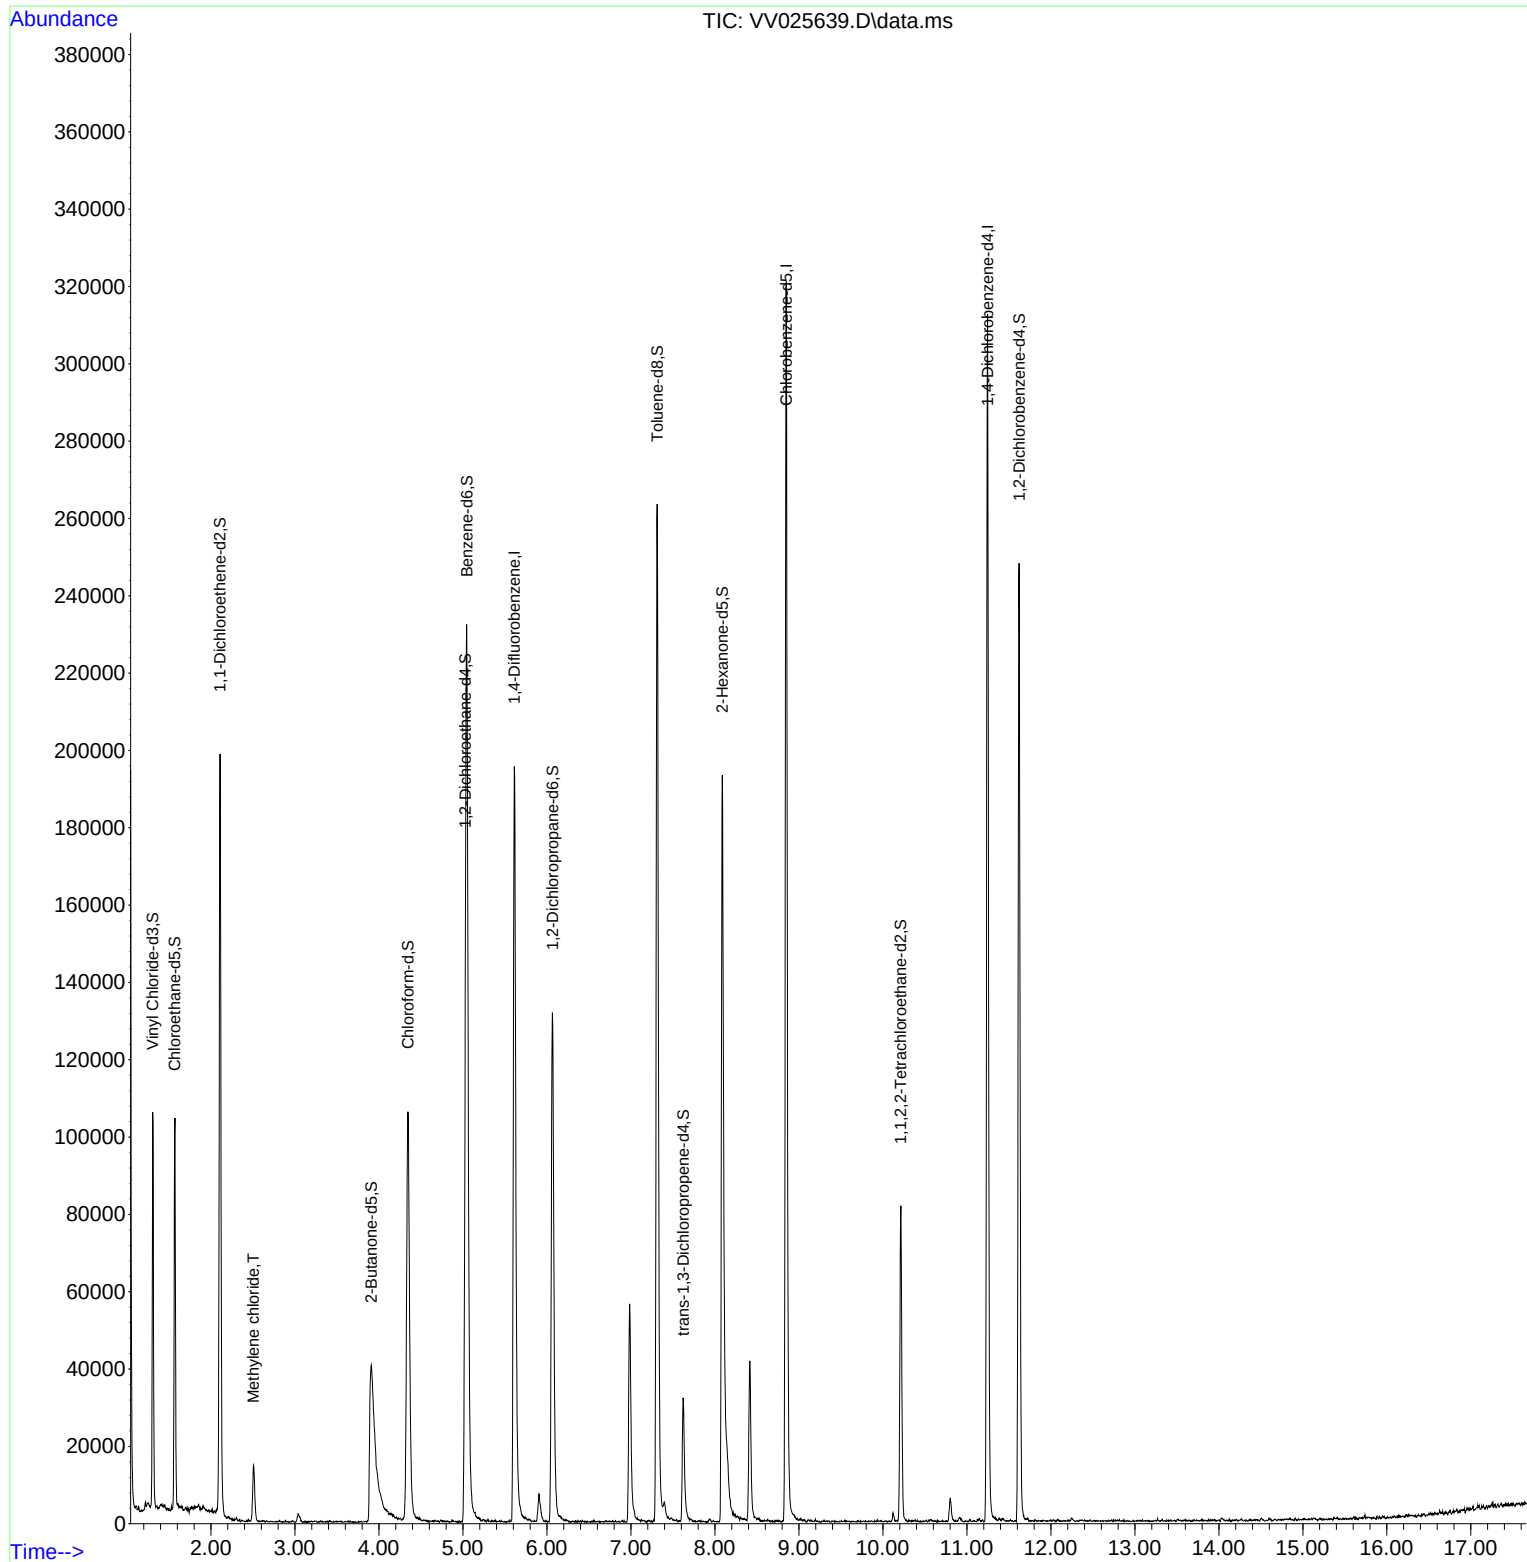

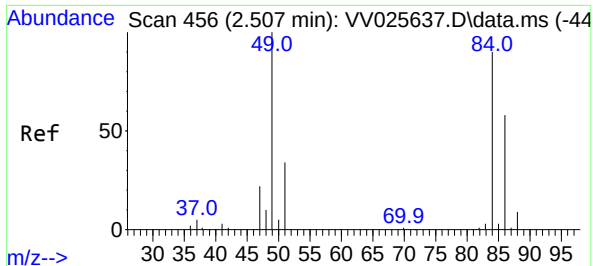

#16  
Methylene chloride  
Concen: 0.436 ug/L  
RT: 2.507 min Scan# 4  
Delta R.T. 0.000 min  
Lab File: VV025639.D  
Acq: 20 Apr 2022 10:53

Instrument :  
MSVOA\_V  
ClientSampleId :  
VHBLK001

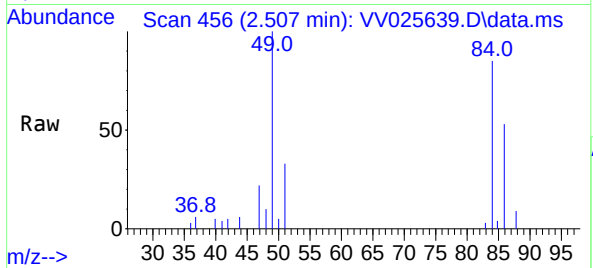

Tgt Ion: 84 Resp: 6378

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 86  | 63.0  | 45.9  | 85.3  |
| 49  | 117.8 | 76.6  | 142.3 |

