

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025638.D
 Acq On : 20 Apr 2022 10:17
 Operator : SY/MD
 Sample : VV0420WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK348

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	91	rBV	92491	92949	18.14%	2.147%
2	1.565	155	163	177	rVB	86968	98201	19.17%	2.268%
3	2.102	319	330	352	rVB	184264	273457	53.38%	6.317%
4	2.507	447	456	465	rVB7	3285	5932	1.16%	0.137%
5	3.912	876	893	926	rBV3	34539	161022	31.43%	3.720%
6	4.343	1010	1027	1054	rBV	91019	232624	45.41%	5.373%
7	5.040	1229	1244	1274	rBV3	203624	512283	100.00%	11.833%
8	5.613	1406	1422	1452	rBV	175698	364549	71.16%	8.421%
9	5.905	1503	1513	1531	rVB6	6704	14379	2.81%	0.332%
10	6.063	1548	1562	1591	rBV2	116700	246786	48.17%	5.701%
11	6.982	1837	1848	1872	rBV	49429	94411	18.43%	2.181%
12	7.314	1938	1951	1970	rBV	232786	415595	81.13%	9.600%
13	7.622	2038	2047	2066	rBV2	27605	51125	9.98%	1.181%
14	8.088	2182	2192	2228	rBV	162847	363690	70.99%	8.401%
15	8.416	2284	2294	2312	rBV2	38312	67506	13.18%	1.559%
16	8.850	2417	2429	2450	rBV	279267	466868	91.13%	10.784%
17	10.214	2842	2853	2869	rBV	70264	112464	21.95%	2.598%
18	10.799	3024	3035	3043	rBV5	3353	6066	1.18%	0.140%
19	11.246	3162	3174	3198	rBV	267966	415943	81.19%	9.608%
20	11.622	3277	3291	3305	rBV	212807	333250	65.05%	7.698%


Sum of corrected areas: 4329100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025638.D
Acq On : 20 Apr 2022 10:17
Operator : SY/MD
Sample : VV0420WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

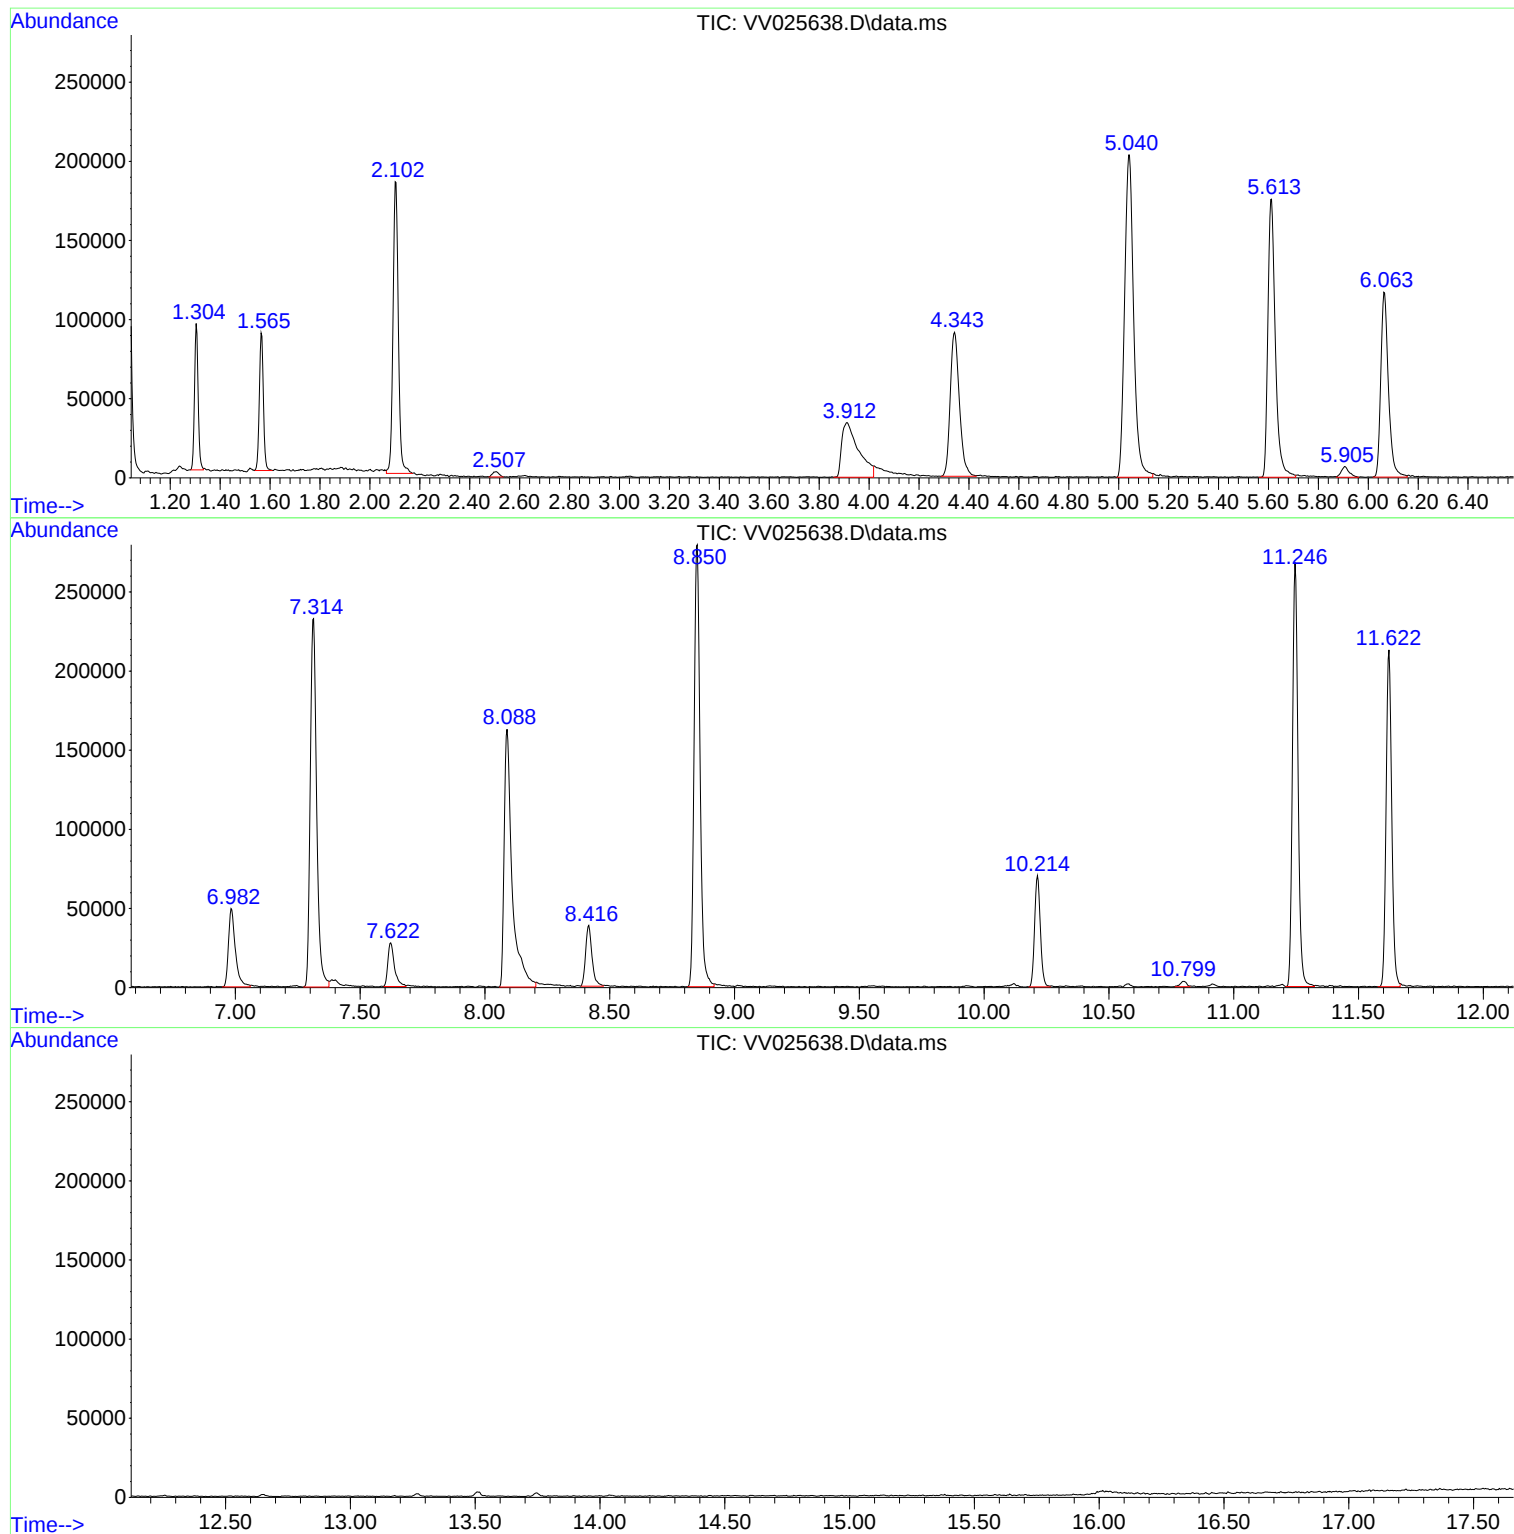

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025638.D
Acq On : 20 Apr 2022 10:17
Operator : SY/MD
Sample : VV0420WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK348










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.416	0.72 ug/L	67506	Chlorobenzene-d5	8.850

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Methoxy-3-methylbenzamide, N,N...	193	C11H15NO2	1369798-01-5	32		
2	Silane, diethoxymethyloctadecyl-	386	C23H50O2Si	067859-75-0	25		
3	Silane, diethoxydimethyl-	148	C6H16O2Si	000078-62-6	25		
4	1H-Indole-3-thiol	149	C8H7NS	000480-94-4	25		
5	4-Ethylbenzoic acid, 2-ethoxyeth...	222	C13H18O3	1000331-30-9	17		

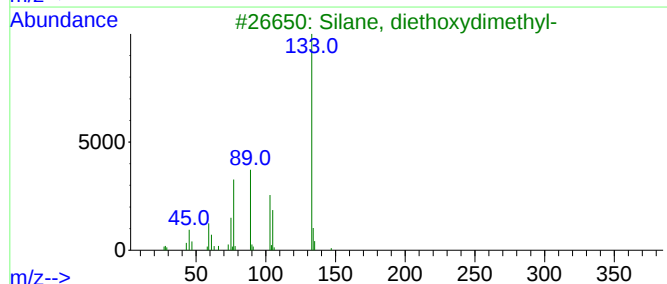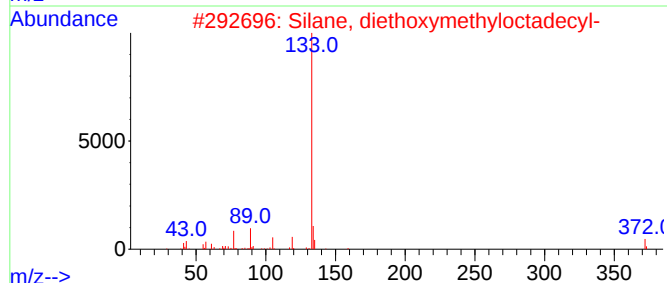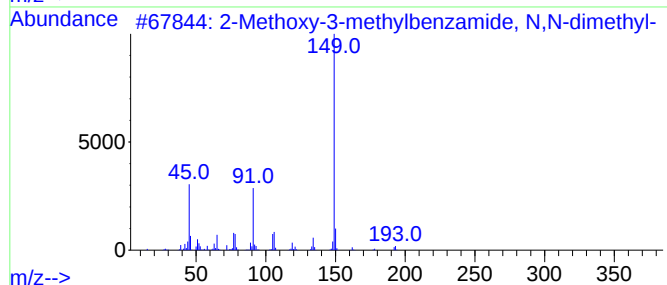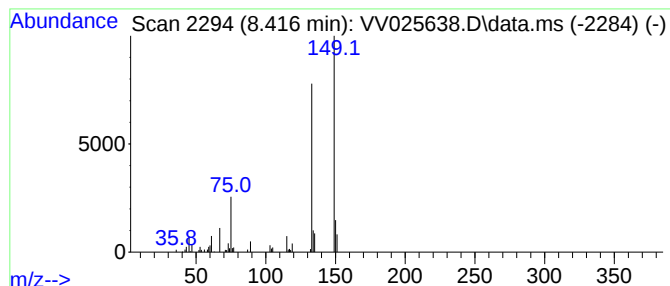

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025638.D
Acq On : 20 Apr 2022 10:17
Operator : SY/MD
Sample : VV0420WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.416	0.7	ug/L	67506	2	8.850	466868	5.0