

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025639.D
 Acq On : 20 Apr 2022 10:53
 Operator : SY/MD
 Sample : N2384-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	102194	104428	17.96%	2.113%
2	1.571	157	165	173	rBV	100869	111760	19.22%	2.261%
3	2.108	322	332	350	rVB	197193	286532	49.28%	5.798%
4	2.507	445	456	471	rBV3	14394	24796	4.26%	0.502%
5	3.908	880	892	945	rBV3	40209	195649	33.65%	3.959%
6	4.346	1006	1028	1056	rBV	105649	267294	45.97%	5.408%
7	5.043	1229	1245	1274	rBV2	232066	581399	100.00%	11.764%
8	5.613	1407	1422	1450	rBV	195356	408209	70.21%	8.259%
9	5.905	1504	1513	1530	rBV5	7151	14798	2.55%	0.299%
10	6.066	1551	1563	1587	rBV2	131746	281026	48.34%	5.686%
11	6.986	1836	1849	1874	rBV	56503	109497	18.83%	2.215%
12	7.313	1940	1951	1971	rBV	263056	471701	81.13%	9.544%
13	7.622	2038	2047	2066	rBV2	31888	59249	10.19%	1.199%
14	8.088	2181	2192	2231	rBV	193158	417211	71.76%	8.442%
15	8.416	2283	2294	2310	rBV2	41338	72308	12.44%	1.463%
16	8.850	2417	2429	2454	rBV	320614	528294	90.87%	10.689%
17	10.214	2840	2853	2871	rBV	81594	128840	22.16%	2.607%
18	10.802	3025	3036	3046	rBV2	6040	10261	1.76%	0.208%
19	11.246	3162	3174	3195	rBV	312342	478361	82.28%	9.679%
20	11.622	3280	3291	3310	rBV	247950	390707	67.20%	7.905%




Sum of corrected areas: 4942320

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025639.D
Acq On : 20 Apr 2022 10:53
Operator : SY/MD
Sample : N2384-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

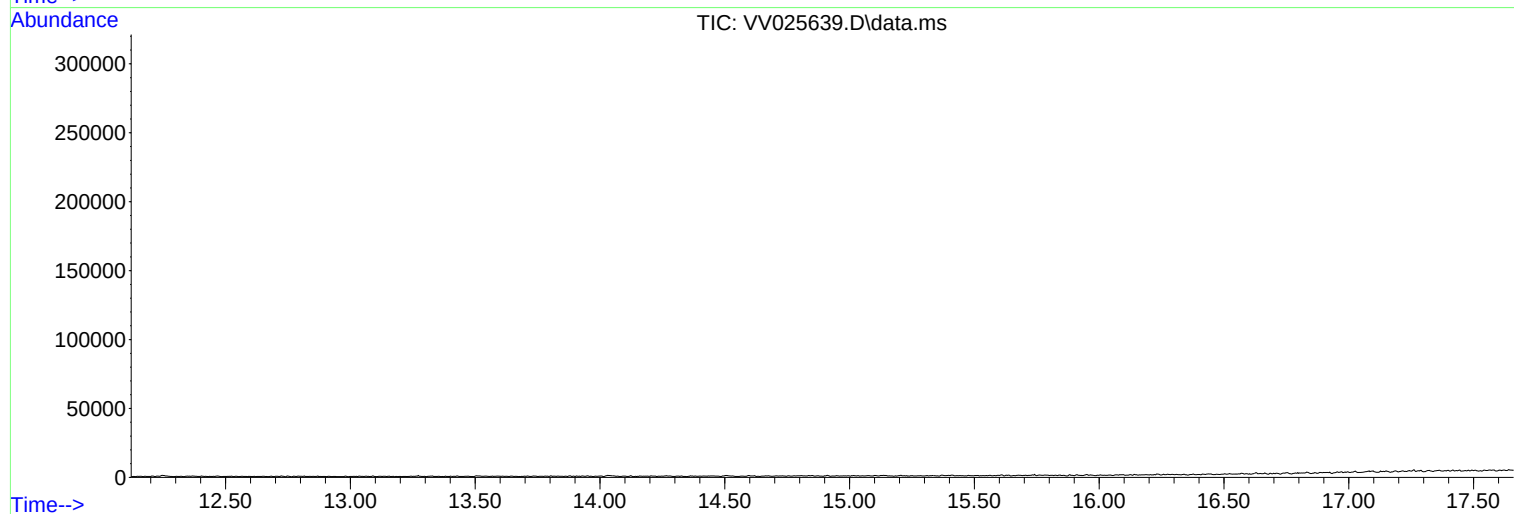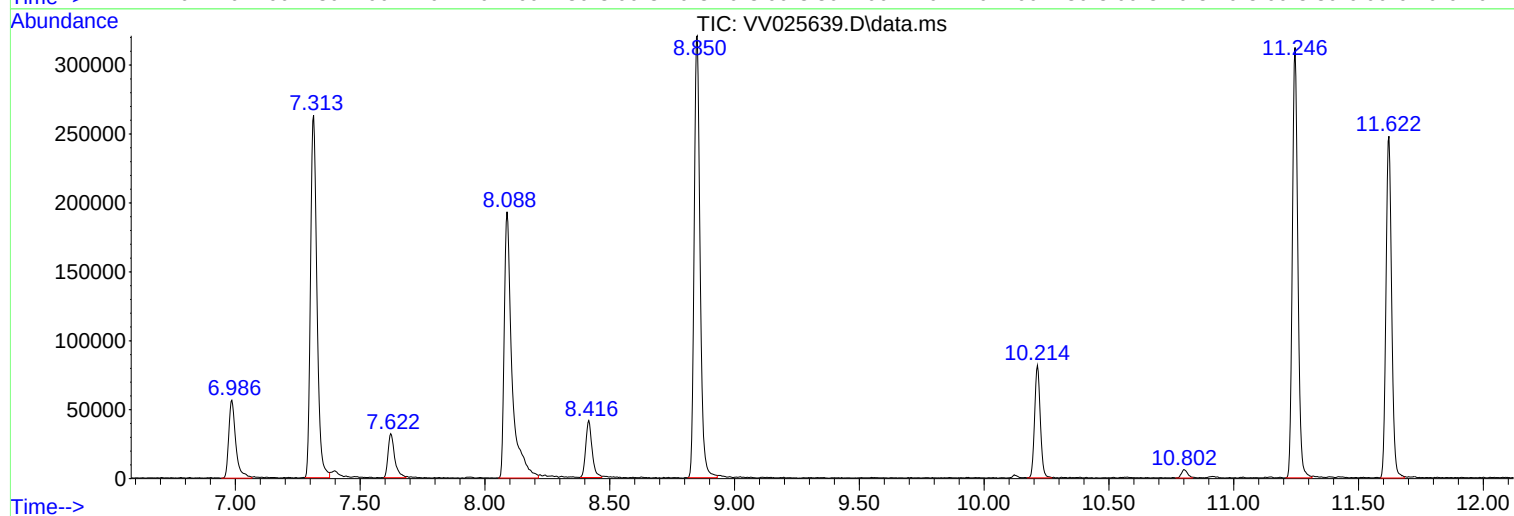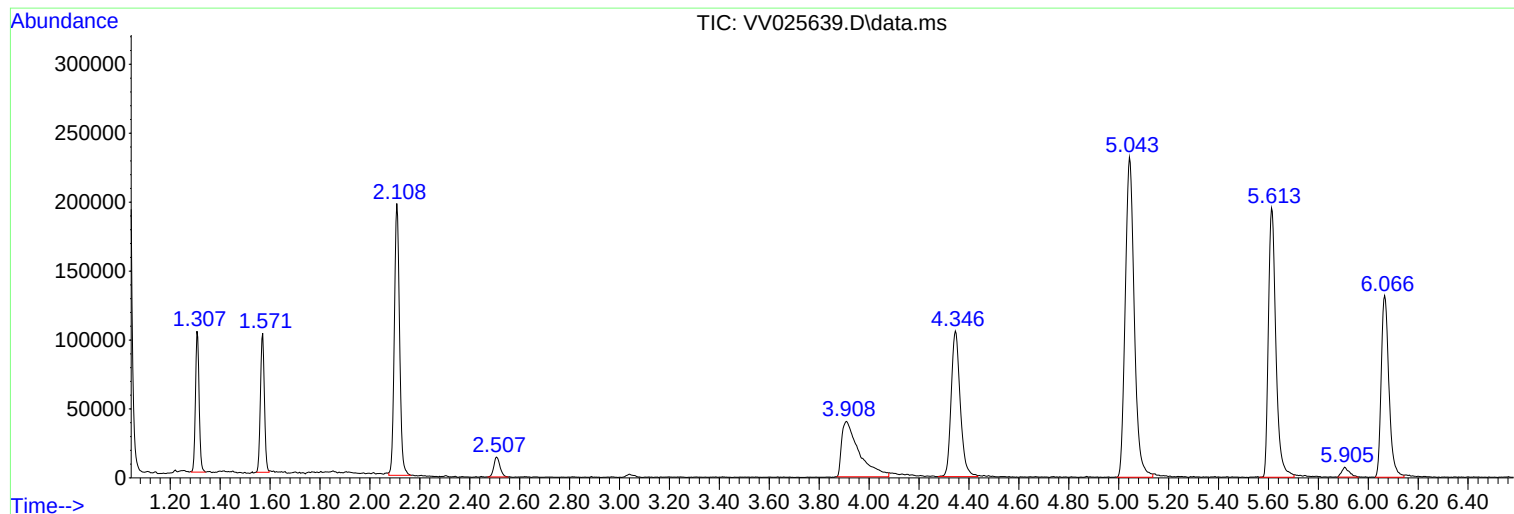

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025639.D
Acq On : 20 Apr 2022 10:53
Operator : SY/MD
Sample : N2384-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 4-Ethylbenzamide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.416	0.68 ug/L	72308	Chlorobenzene-d5	8.850

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Ethylbenzamide	149	C9H11NO	033695-58-8	64
2			1,3-Diisopropoxy-1,3-dimethyl-1,...	232	C10H24O2Si2	198066-66-9	40
3			Thioglycolic acid, tert-butylidim...	206	C8H18O2SSi	1000476-01-2	38
4			Silane, dodecyldiethoxymethyl-	302	C17H38O2Si	060317-40-0	35
5			4-Ethylbenzoic acid, cyclohexyl ...	232	C15H20O2	1000293-32-1	25

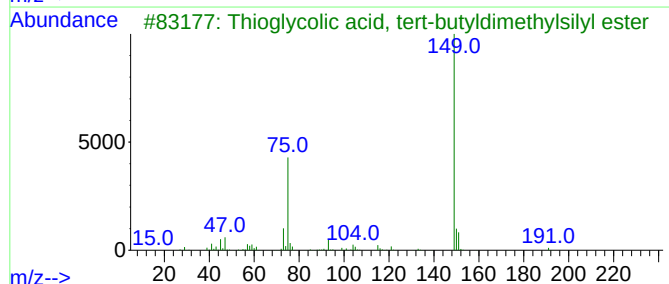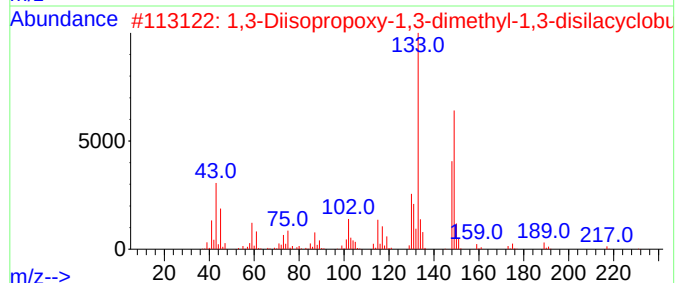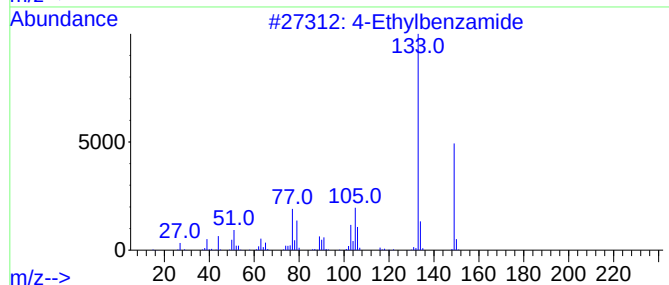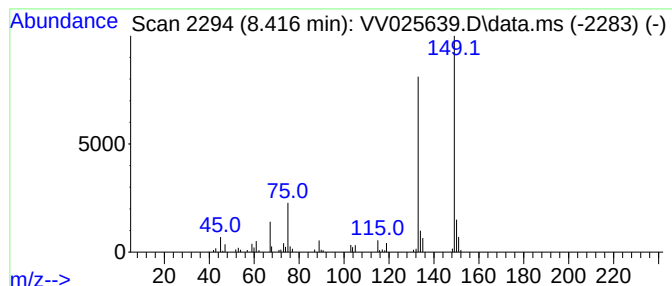

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025639.D
Acq On : 20 Apr 2022 10:53
Operator : SY/MD
Sample : N2384-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
4-Ethylbenzamide	8.416	0.7	ug/L	72308	2	8.850	528294	5.0