

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025641.D
 Acq On : 20 Apr 2022 13:16
 Operator : SY/MD
 Sample : N2471-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	93	rVB	85831	87656	17.42%	2.150%
2	1.571	157	165	177	rBV	87671	100997	20.07%	2.477%
3	2.111	322	333	350	rBV	163741	238433	47.39%	5.847%
4	3.905	882	891	892	rBV	34635	40907	8.13%	1.003%
5	4.352	1015	1030	1063	rVB	94688	249343	49.56%	6.115%
6	5.050	1230	1247	1269	rBV2	202285	503142	100.00%	12.339%
7	5.619	1411	1424	1447	rBV2	162934	336340	66.85%	8.249%
8	5.912	1499	1515	1527	rBV5	6580	13578	2.70%	0.333%
9	6.072	1548	1565	1592	rBV2	118474	249393	49.57%	6.116%
10	6.989	1840	1850	1877	rBV	49681	93748	18.63%	2.299%
11	7.317	1939	1952	1971	rBV	232679	414886	82.46%	10.175%
12	7.400	1972	1978	1990	rVB3	6736	12095	2.40%	0.297%
13	7.625	2038	2048	2074	rBV2	27265	51927	10.32%	1.273%
14	8.092	2182	2193	2225	rBV	176252	359964	71.54%	8.828%
15	8.850	2417	2429	2448	rBV	268107	439759	87.40%	10.785%
16	10.214	2840	2853	2870	rBV	69944	112269	22.31%	2.753%
17	10.381	2896	2905	2916	rVB4	4611	7285	1.45%	0.179%
18	11.246	3164	3174	3192	rBV	258008	399946	79.49%	9.808%
19	11.535	3255	3264	3273	rBV7	3173	5702	1.13%	0.140%
20	11.622	3279	3291	3308	rBV	214290	340320	67.64%	8.346%
21	12.345	3503	3516	3528	rBV6	11565	19887	3.95%	0.488%


Sum of corrected areas: 4077577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025641.D
Acq On : 20 Apr 2022 13:16
Operator : SY/MD
Sample : N2471-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

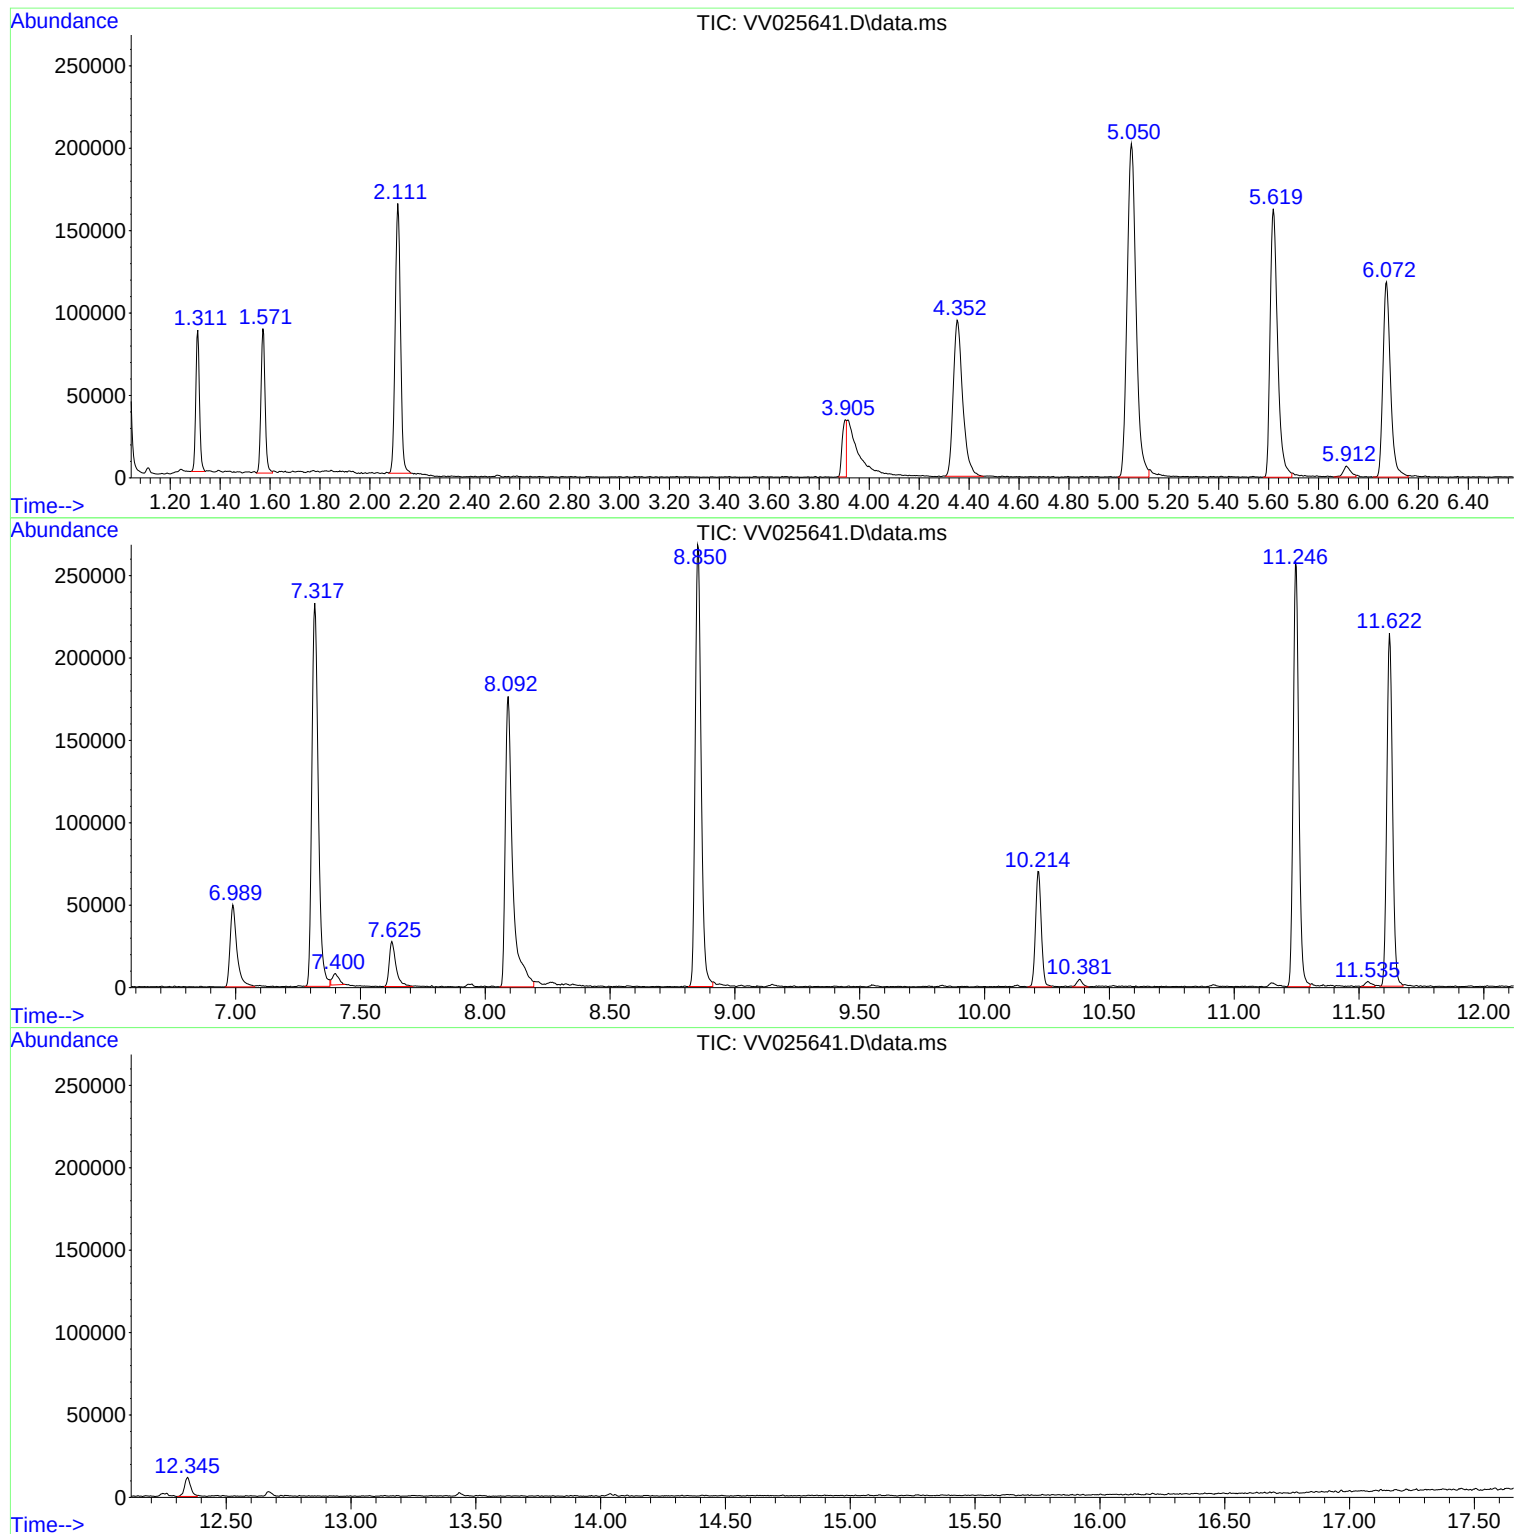

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025641.D
Acq On : 20 Apr 2022 13:16
Operator : SY/MD
Sample : N2471-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025641.D
Acq On : 20 Apr 2022 13:16
Operator : SY/MD
Sample : N2471-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc