

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025648.D
 Acq On : 20 Apr 2022 16:00
 Operator : SY/MD
 Sample : VIBLK246
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK246

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	93	rVB	76113	77633	16.32%	1.992%
2	1.574	158	166	176	rBV	77916	89495	18.81%	2.296%
3	2.114	323	334	352	rVB	145218	214677	45.12%	5.508%
4	2.513	449	458	468	rVB5	4341	7784	1.64%	0.200%
5	3.899	877	889	923	rBV2	45490	158954	33.41%	4.078%
6	4.352	1014	1030	1060	rBV	89438	226283	47.56%	5.806%
7	5.050	1232	1247	1273	rBV2	192184	475799	100.00%	12.208%
8	5.619	1411	1424	1448	rBV	143647	295155	62.03%	7.573%
9	5.911	1502	1515	1533	rVB5	6167	13495	2.84%	0.346%
10	6.072	1553	1565	1592	rBV	112276	236942	49.80%	6.079%
11	6.989	1838	1850	1868	rBV	46686	86333	18.14%	2.215%
12	7.317	1941	1952	1972	rBV	215796	386895	81.31%	9.927%
13	7.625	2039	2048	2073	rBV2	25019	49869	10.48%	1.280%
14	7.979	2150	2158	2172	rVB3	19527	33436	7.03%	0.858%
15	8.091	2182	2193	2233	rBV	168984	351247	73.82%	9.012%
16	8.423	2287	2296	2304	rBV4	4043	5999	1.26%	0.154%
17	8.853	2417	2430	2461	rBV	237004	394452	82.90%	10.121%
18	10.217	2841	2854	2871	rBV	67791	109486	23.01%	2.809%
19	10.381	2896	2905	2914	rBV4	3575	5402	1.14%	0.139%
20	11.249	3164	3175	3194	rBV	224750	353890	74.38%	9.080%
21	11.622	3277	3291	3310	rBV	206222	324312	68.16%	8.321%




Sum of corrected areas: 3897538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025648.D
Acq On : 20 Apr 2022 16:00
Operator : SY/MD
Sample : VIBLK246
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

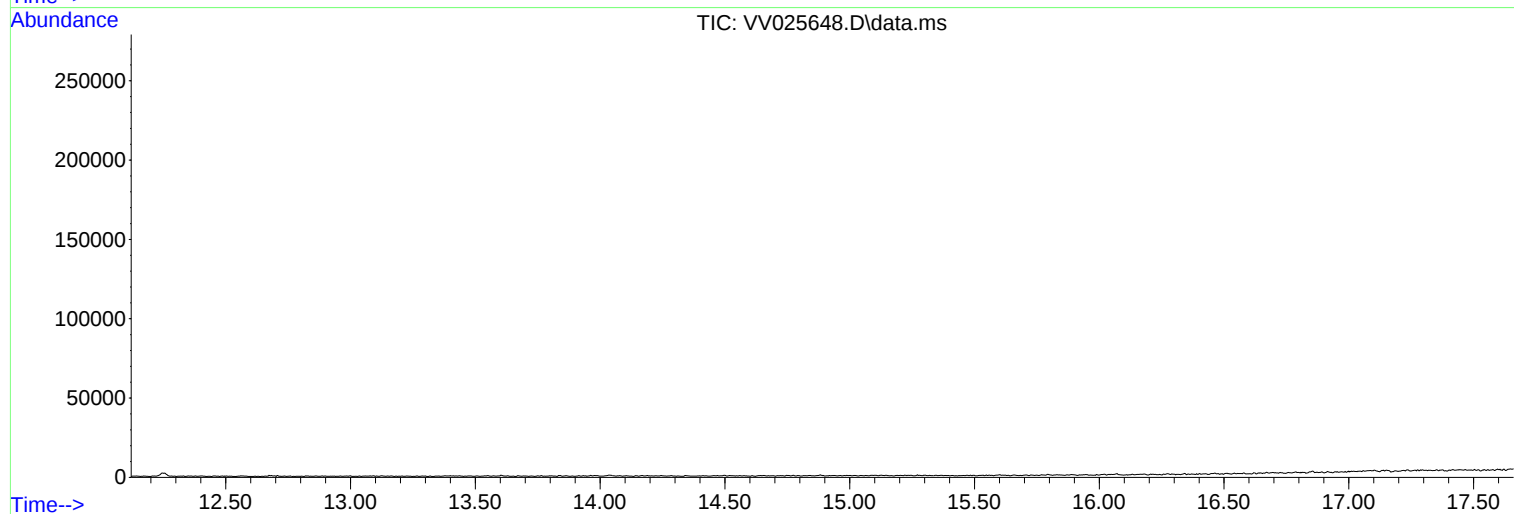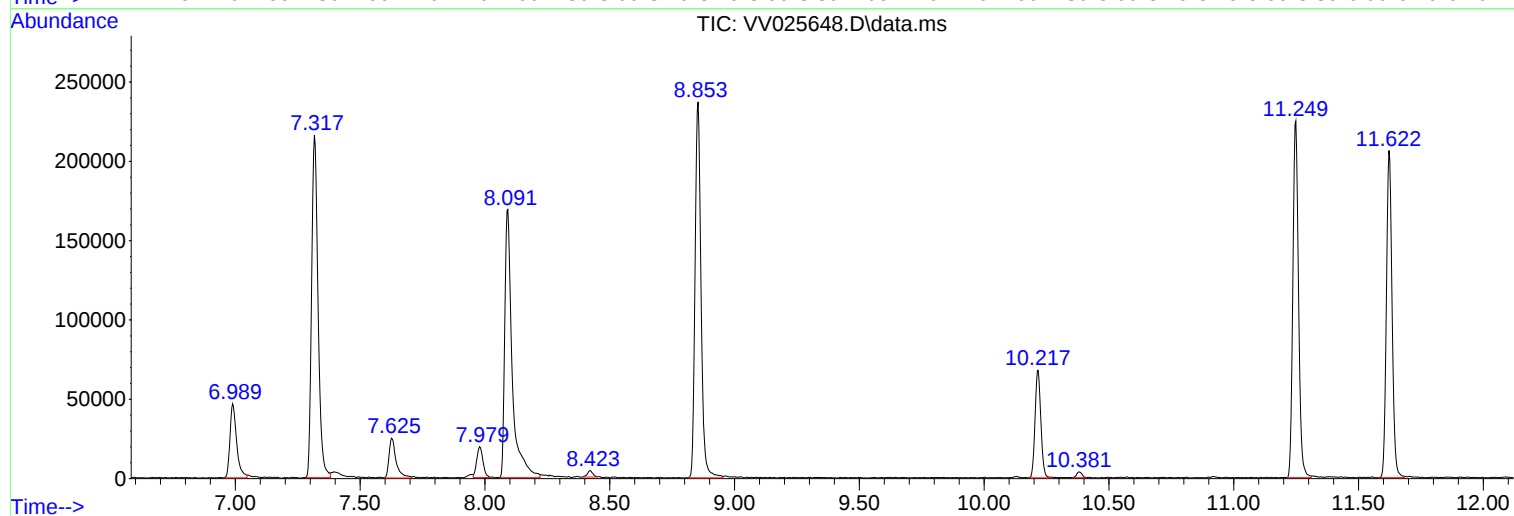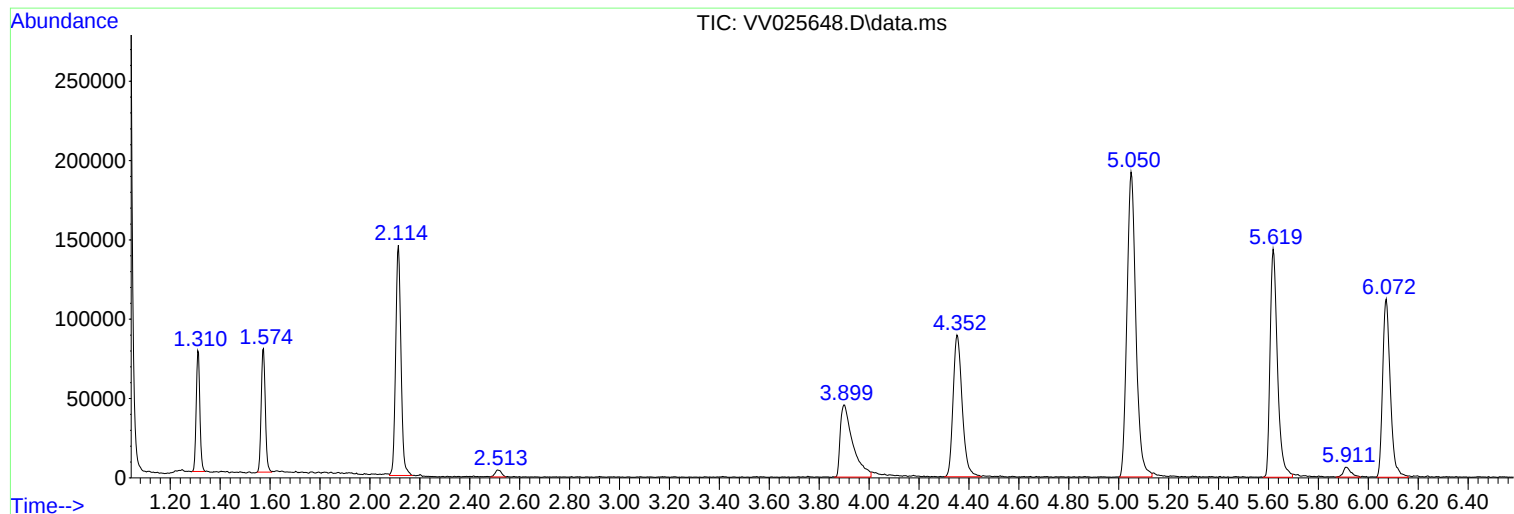

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025648.D
Acq On : 20 Apr 2022 16:00
Operator : SY/MD
Sample : VIBLK246
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025648.D
Acq On : 20 Apr 2022 16:00
Operator : SY/MD
Sample : VIBLK246
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc