

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025656.D
 Acq On : 20 Apr 2022 19:07
 Operator : SY/MD
 Sample : N2492-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	95	rVB	77359	79232	17.31%	2.032%
2	1.571	158	165	175	rBV	73907	85178	18.60%	2.185%
3	2.111	323	333	351	rVB	140904	211398	46.17%	5.422%
4	2.513	446	458	473	rBV2	10295	17538	3.83%	0.450%
5	2.963	587	598	614	rBV3	3141	7617	1.66%	0.195%
6	3.911	883	893	933	rBV2	29778	133712	29.21%	3.430%
7	4.355	1014	1031	1060	rBV3	89214	264656	57.81%	6.788%
8	5.053	1233	1248	1280	rBV2	180279	457826	100.00%	11.743%
9	5.619	1413	1424	1450	rBV	137424	286120	62.50%	7.339%
10	5.915	1502	1516	1530	rBV8	6244	13974	3.05%	0.358%
11	6.072	1552	1565	1587	rBV2	107192	223102	48.73%	5.722%
12	6.989	1840	1850	1870	rBV2	42798	83046	18.14%	2.130%
13	7.316	1938	1952	1970	rBV	203898	362515	79.18%	9.298%
14	7.628	2039	2049	2066	rBV	24303	46237	10.10%	1.186%
15	7.979	2147	2158	2178	rVB2	48561	86730	18.94%	2.225%
16	8.091	2182	2193	2228	rBV	162158	346568	75.70%	8.889%
17	8.853	2419	2430	2449	rBV	231644	374462	81.79%	9.605%
18	10.217	2842	2854	2869	rBV	65200	103183	22.54%	2.647%
19	10.377	2894	2904	2918	rVB4	4476	8351	1.82%	0.214%
20	11.249	3164	3175	3194	rBV	207546	325554	71.11%	8.350%
21	11.532	3253	3263	3278	rBV2	17590	31382	6.85%	0.805%
22	11.622	3280	3291	3314	rVB	194836	306507	66.95%	7.862%
23	12.246	3477	3485	3496	rVB6	3481	5162	1.13%	0.132%
24	12.345	3507	3516	3524	rBV7	6517	10111	2.21%	0.259%
25	13.432	3848	3854	3861	rBV8	3589	4937	1.08%	0.127%
26	17.094	4983	4993	5002	rBV	15420	23692	5.17%	0.608%




Sum of corrected areas: 3898790

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025656.D
Acq On : 20 Apr 2022 19:07
Operator : SY/MD
Sample : N2492-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

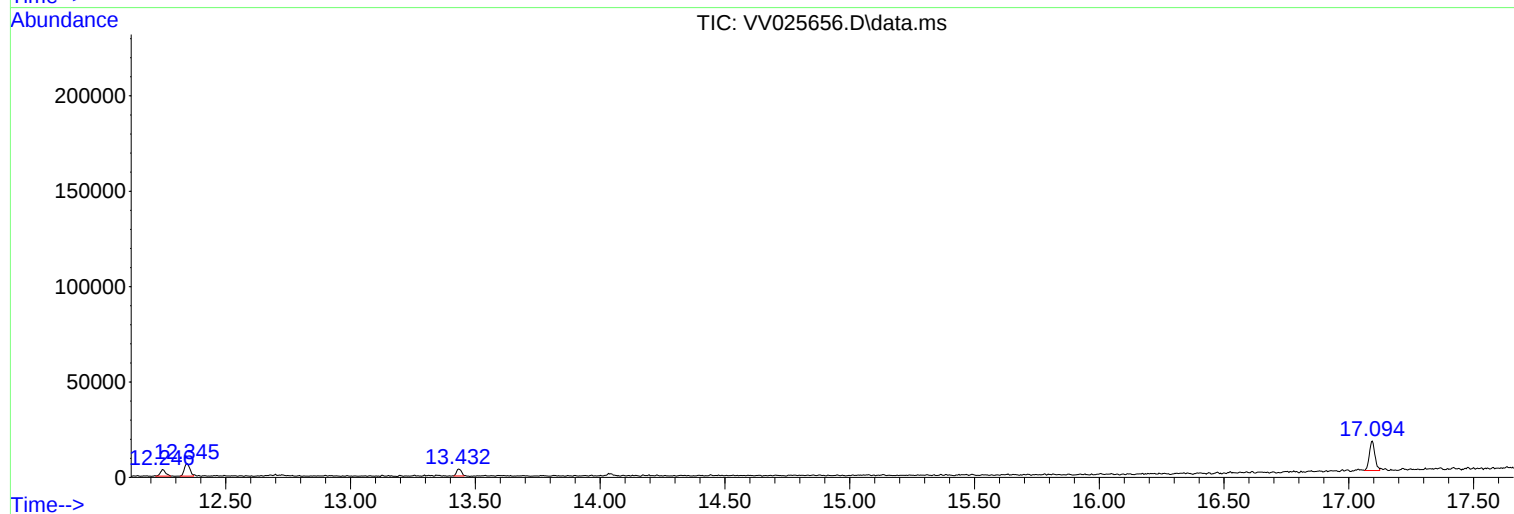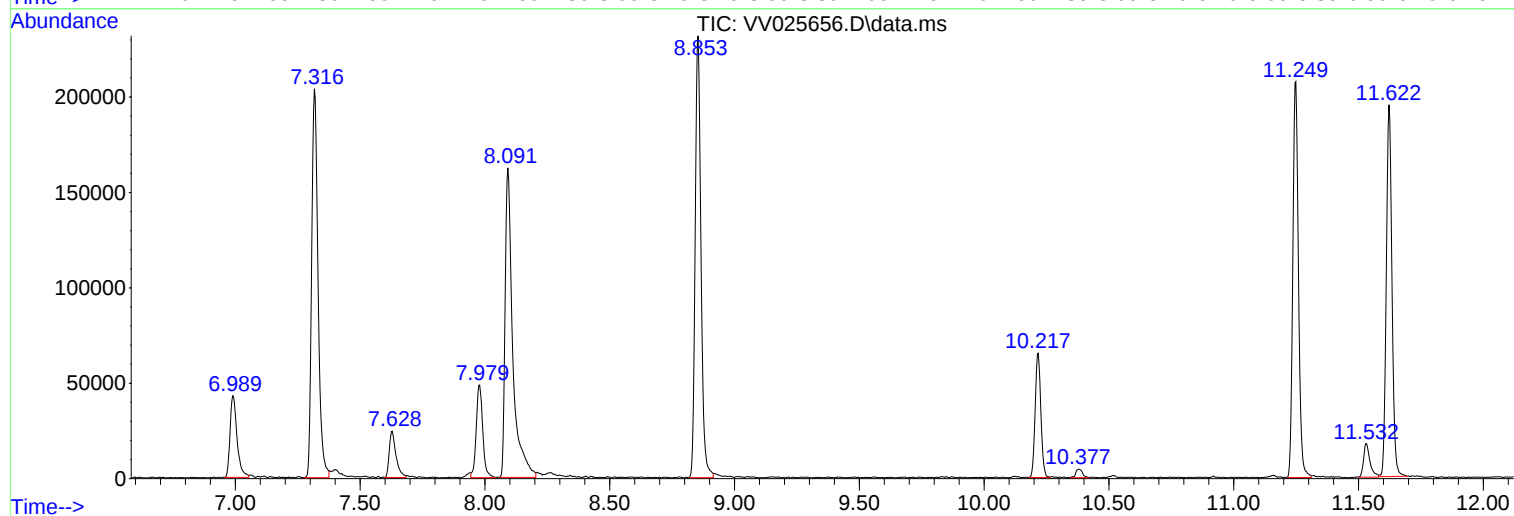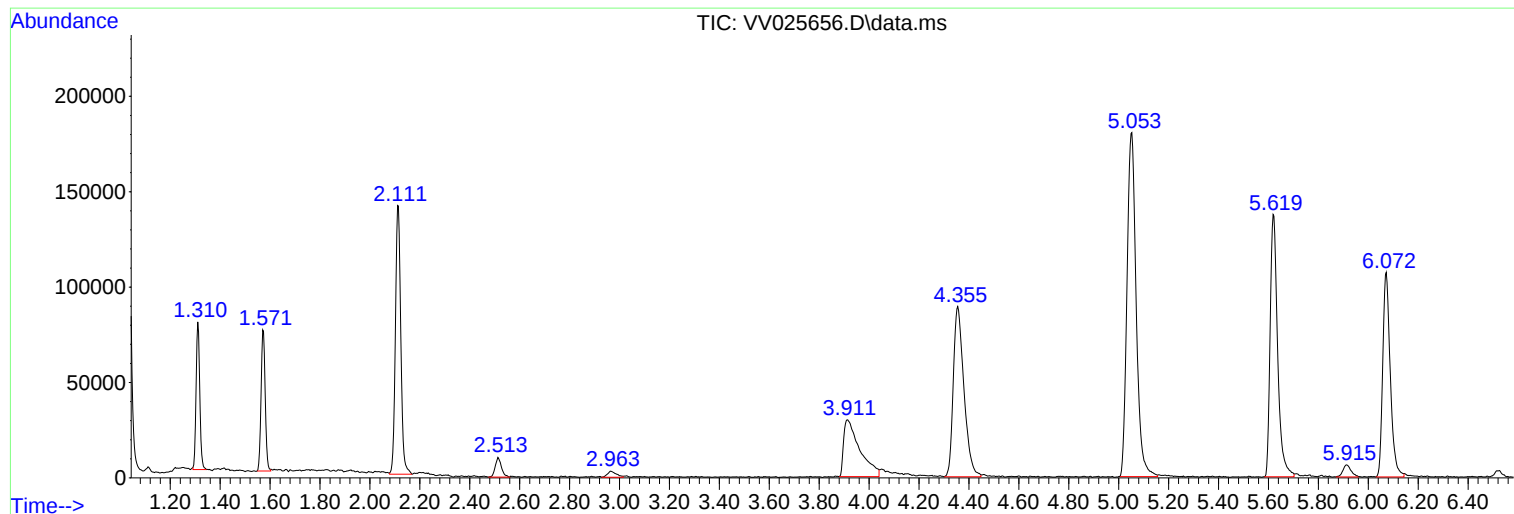

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025656.D
Acq On : 20 Apr 2022 19:07
Operator : SY/MD
Sample : N2492-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
Data File : VV025656.D
Acq On : 20 Apr 2022 19:07
Operator : SY/MD
Sample : N2492-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc