


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042022\
 Data File : VV025636.D
 Acq On : 20 Apr 2022 09:01
 Operator : SY/MD
 Sample : BFB306
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB306

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Apr 23 01:57:52 2022

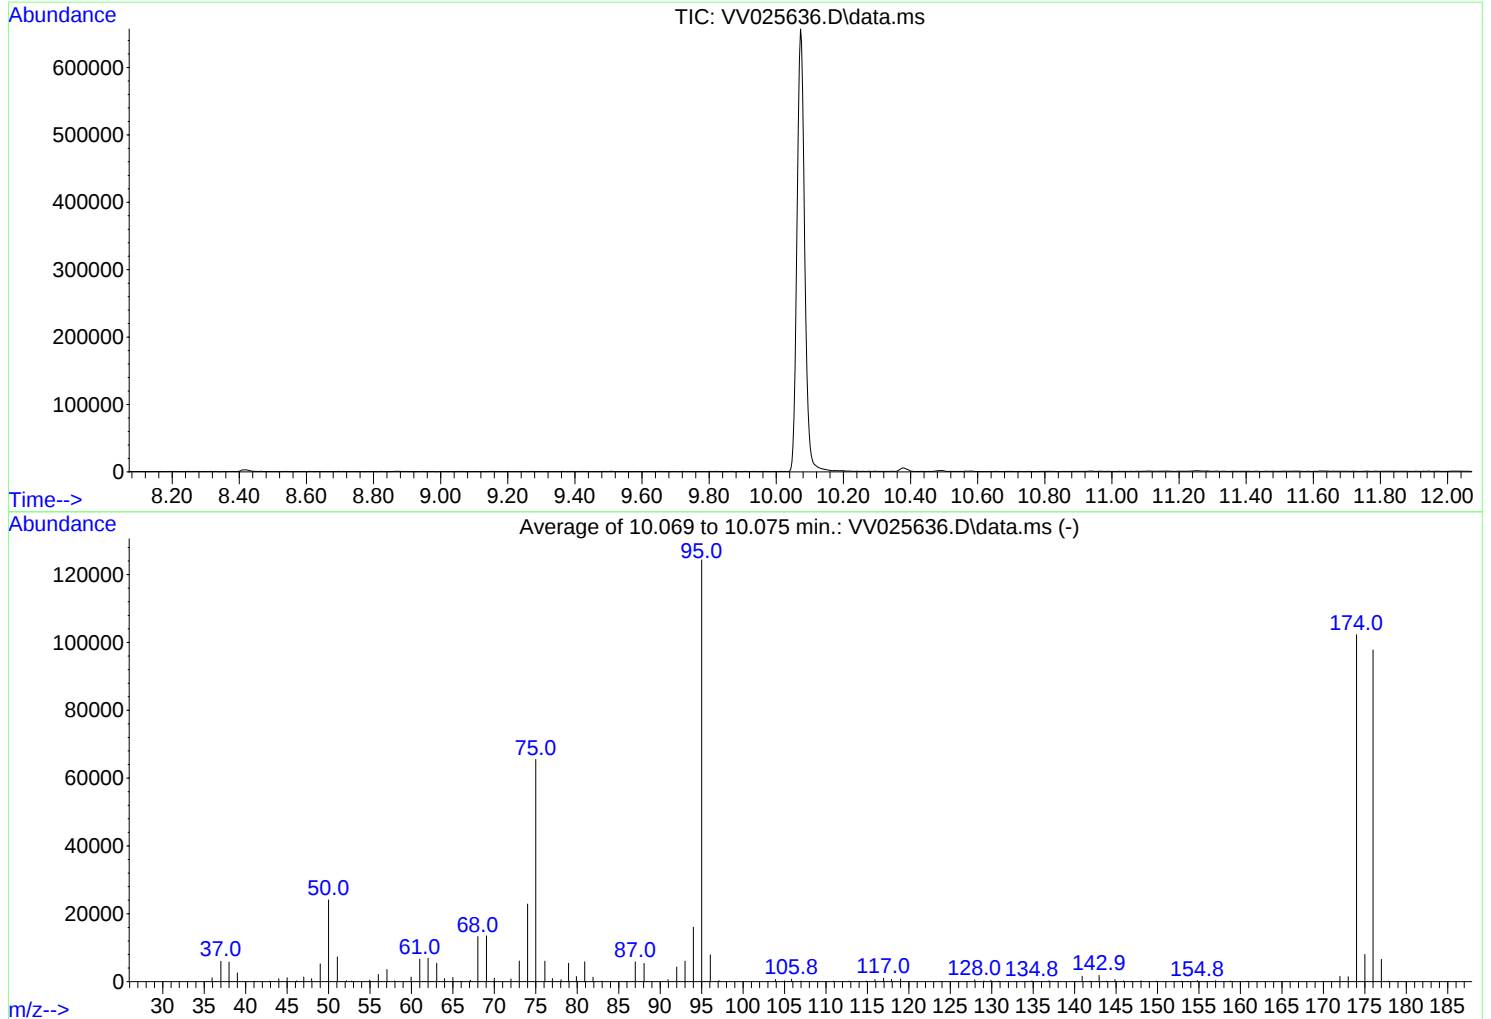

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	24125	PASS
75	95	30	80	52.7	65517	PASS
95	95	100	100	100.0	124357	PASS
96	95	5	9	6.3	7869	PASS
173	174	0.00	2	1.4	1466	PASS
174	95	50	120	82.3	102291	PASS
175	174	5	9	7.8	8012	PASS
176	174	95	105	95.6	97803	PASS
177	176	5	10	6.7	6543	PASS

m/z	Abundance
39.90	252.0
44.00	291.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
36.00	1125.0
37.00	5944.0
38.00	5707.0
39.00	2639.0
40.00	302.0
41.10	120.0
42.90	172.0
44.00	1113.0
45.00	1137.0
46.20	224.0
47.00	1479.0
47.90	837.0
49.00	5282.0
50.00	23880.0
51.10	6985.0
52.10	279.0
52.80	212.0
53.90	121.0
55.00	461.0
56.00	2099.0
57.10	3407.0
57.90	214.0
60.00	1325.0
61.00	6666.0
62.00	6674.0
63.00	5395.0
64.00	813.0
65.00	1133.0
65.90	151.0
67.10	402.0
68.00	12506.0
69.00	13177.0
70.00	1057.0
72.00	824.0
73.00	6016.0
74.00	22000.0
75.00	64488.0
76.10	5857.0
77.00	829.0
78.10	534.0
78.90	5448.0
79.90	1518.0
80.90	5668.0
81.90	1228.0
83.00	171.0
87.00	5457.0
88.00	5184.0
91.00	605.0
92.00	4108.0
93.00	5592.0
94.00	15007.0
95.00	120144.0
96.00	7825.0
97.10	362.0
103.90	665.0
105.00	225.0
105.80	749.0
107.00	189.0
108.10	108.0
109.90	121.0
110.90	184.0
112.00	124.0
112.80	202.0
114.90	183.0
115.90	595.0
117.00	919.0
117.90	623.0
119.00	752.0
128.00	477.0
129.00	204.0
129.80	418.0
130.80	188.0
134.80	252.0
136.90	293.0
140.90	1611.0
141.80	136.0
142.90	1940.0
143.90	160.0
144.90	601.0
145.90	245.0
146.80	102.0
148.00	313.0
149.90	214.0
152.00	125.0
152.90	123.0
154.80	291.0
155.90	118.0
157.00	244.0
158.80	187.0
160.80	148.0
172.00	1484.0
173.00	1378.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

174.00	96624.0
175.00	7669.0
176.00	92832.0
177.00	6225.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
36.00	1149.0
37.00	6215.0
38.00	5961.0
39.00	2673.0
39.90	319.0
41.10	165.0
42.80	153.0
44.00	1192.0
45.00	1191.0
46.10	291.0
47.00	1419.0
47.90	898.0
49.00	5444.0
50.00	24904.0
51.10	7521.0
52.20	294.0
52.80	173.0
53.90	119.0
55.00	481.0
56.00	2236.0
57.10	3701.0
58.00	235.0
60.00	1362.0
61.00	6924.0
62.00	7178.0
63.00	5590.0
64.00	914.0
65.00	1275.0
66.10	152.0
67.10	456.0
68.00	13631.0
69.10	13962.0
70.00	1077.0
71.00	113.0
72.00	843.0
73.00	6345.0
74.00	23680.0
75.00	67808.0
76.10	6241.0
77.00	943.0
78.00	572.0
79.00	5652.0
79.90	1563.0
80.90	6118.0
81.90	1406.0
83.00	183.0
85.80	122.0
87.00	6025.0
88.10	5606.0
90.90	654.0
92.00	4466.0
93.00	6268.0
94.00	16624.0
95.00	128632.0
96.10	8139.0
97.10	336.0
103.90	661.0
105.00	295.0
105.80	777.0
107.00	192.0
108.10	104.0
109.90	105.0
110.90	173.0
112.10	100.0
112.80	215.0
114.90	213.0
115.90	643.0
117.00	992.0
117.90	681.0
119.00	814.0
123.90	122.0
127.90	530.0
129.10	246.0
129.90	433.0
130.80	204.0
134.80	262.0
136.90	307.0
140.90	1660.0
141.80	146.0
142.90	1912.0
143.80	188.0
144.90	666.0
145.90	245.0
146.80	107.0
148.00	313.0
149.90	219.0
152.00	106.0
152.80	138.0
154.80	379.0
155.90	115.0
157.00	267.0
158.80	221.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

160.90	136.0
170.00	110.0
172.00	1604.0
173.00	1517.0
174.00	105264.0
175.00	8217.0
176.00	100944.0
177.00	6802.0
177.90	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

m/z	Abundance
35.90	1103.0
37.00	5825.0
38.00	5659.0
39.00	2536.0
39.90	330.0
41.10	155.0
42.80	102.0
44.00	1131.0
45.00	1193.0
46.10	273.0
47.00	1251.0
48.00	853.0
49.00	5010.0
50.00	23592.0
51.00	7395.0
52.10	335.0
52.90	121.0
54.00	117.0
54.90	447.0
56.00	2095.0
57.00	3693.0
58.00	216.0
59.90	1359.0
61.00	6403.0
62.00	6831.0
63.10	5301.0
64.00	915.0
65.00	1291.0
66.20	137.0
67.10	457.0
68.00	13749.0
69.10	13380.0
70.00	1033.0
70.90	126.0
72.00	757.0
73.00	5968.0
74.00	22976.0
75.00	64256.0
76.10	6020.0
77.00	914.0
78.00	554.0
78.90	5210.0
79.90	1455.0
80.90	5793.0
81.90	1367.0
83.00	207.0
86.00	170.0
87.00	6028.0
88.00	5322.0
90.90	645.0
92.00	4260.0
93.00	6263.0
94.00	16528.0
95.00	124296.0
96.10	7642.0
97.10	239.0
103.90	586.0
105.00	262.0
105.90	685.0
107.00	187.0
107.90	121.0
111.00	184.0
112.10	106.0
112.80	172.0
114.90	197.0
115.90	572.0
116.90	1071.0
117.90	669.0
119.00	782.0
123.80	155.0
127.90	517.0
129.10	282.0
130.00	445.0
130.90	221.0
134.90	275.0
136.90	268.0
140.90	1569.0
141.90	152.0
143.00	1748.0
143.80	189.0
144.80	573.0
145.90	207.0
146.80	126.0
148.00	280.0
149.90	179.0
152.80	139.0
153.70	101.0
154.80	374.0
157.00	289.0
158.80	204.0
161.00	153.0
170.00	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306

171.00	315.0
172.00	1607.0
173.00	1503.0
174.00	104984.0
175.00	8151.0
176.00	99632.0
177.00	6602.0
177.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB306