

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV042122\  
 Data File : VV025660.D  
 Acq On : 21 Apr 2022 12:34  
 Operator : SY/MD  
 Sample : VV0421WBL01  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK349

Quant Time: Apr 22 03:07:33 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Apr 22 03:06:52 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min)  |
|-------------------------------|--------|-------|----------|----------|-------|-----------|
| -----                         |        |       |          |          |       |           |
| Internal Standards            |        |       |          |          |       |           |
| 1) 1,4-Difluorobenzene        | 5.613  | 114   | 183642   | 5.000    | ug/L  | 0.00      |
| 28) Chlorobenzene-d5          | 8.850  | 117   | 184536   | 5.000    | ug/L  | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.246 | 152   | 85687    | 5.000    | ug/L  | 0.00      |
| System Monitoring Compounds   |        |       |          |          |       |           |
| 4) Vinyl Chloride-d3          | 1.311  | 65    | 71643    | 4.196    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 84.000%   |
| 7) Chloroethane-d5            | 1.571  | 69    | 71713    | 3.948    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 79.000%   |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63    | 111693   | 3.266    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 65.400%   |
| 20) 2-Butanone-d5             | 3.889  | 46    | 128183   | 61.721   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 123.440%  |
| 24) Chloroform-d              | 4.346  | 84    | 134667   | 5.220    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 104.400%  |
| 26) 1,2-Dichloroethane-d4     | 5.031  | 65    | 62987    | 5.666    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 113.400%  |
| 32) Benzene-d6                | 5.047  | 84    | 258272   | 4.837    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 96.800%   |
| 36) 1,2-Dichloropropane-d6    | 6.066  | 67    | 79931    | 5.368    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 107.400%  |
| 41) Toluene-d8                | 7.314  | 98    | 221315   | 4.467    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 89.400%   |
| 43) trans-1,3-Dichloroprop... | 7.622  | 79    | 23277    | 4.651    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 93.000%   |
| 46) 2-Hexanone-d5             | 8.085  | 63    | 90832    | 51.709   | ug/L  | 0.00      |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 103.420%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214 | 84    | 47374    | 5.036    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 100.800%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152   | 74845    | 5.210    | ug/L  | 0.00      |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 104.200%  |
| Target Compounds              |        |       |          |          |       |           |
| 16) Methylene chloride        | 2.507  | 84    | 5177     | 0.335    | ug/L  | Qvalue 91 |
| -----                         |        |       |          |          |       |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV042122\  
Data File : VV025660.D  
Acq On : 21 Apr 2022 12:34  
Operator : SY/MD  
Sample : VV0421WBL01  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK349


Quant Time: Apr 22 03:07:33 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR040822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Apr 22 03:06:52 2022  
Response via : Initial Calibration

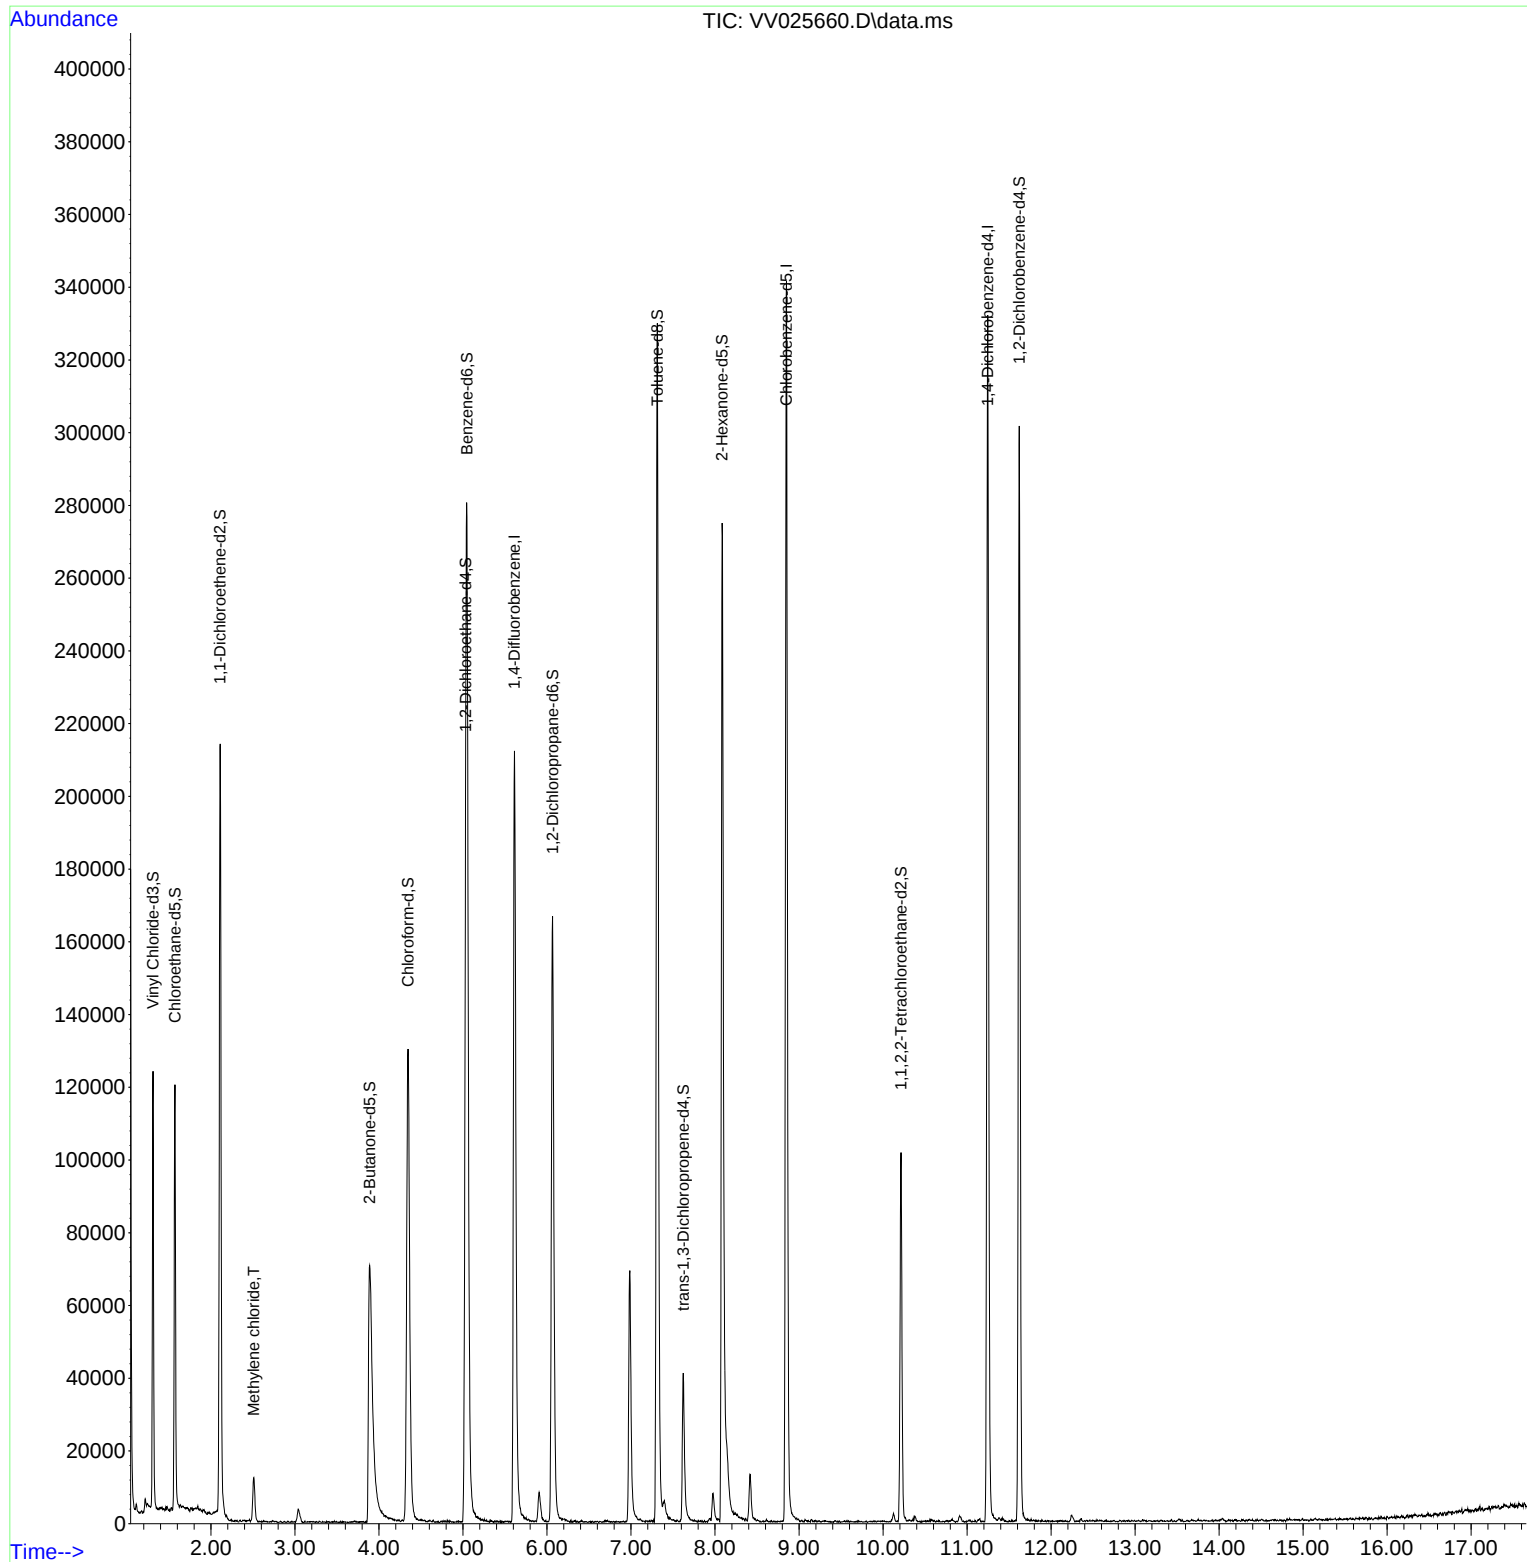

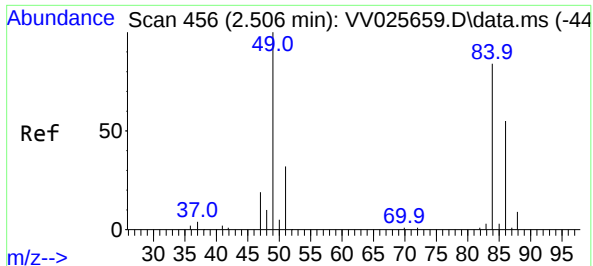

#16  
Methylene chloride  
Concen: 0.335 ug/L  
RT: 2.507 min Scan# 4  
Delta R.T. 0.000 min  
Lab File: VV025660.D  
Acq: 21 Apr 2022 12:34

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK349

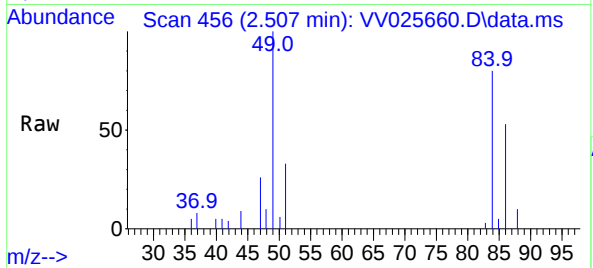

Tgt Ion: 84 Resp: 5177

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 86  | 65.3  | 45.9  | 85.3  |
| 49  | 124.4 | 76.6  | 142.3 |

