

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042122\
 Data File : VW025665.D
 Acq On : 21 Apr 2022 14:37
 Operator : SY/MD
 Sample : N2492-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T7

Quant Time: Apr 22 03:08:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 22 03:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	150241	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	154863	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	68134	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	55820	3.996	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.574	69	58029	3.905	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.200%
11) 1,1-Dichloroethene-d2	2.114	63	88776	3.173	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%
20) 2-Butanone-d5	3.895	46	112113	65.985	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.960%#
24) Chloroform-d	4.352	84	114262	5.413	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.200%
26) 1,2-Dichloroethane-d4	5.037	65	54512	5.994	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	119.800%
32) Benzene-d6	5.053	84	218890	4.885	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
36) 1,2-Dichloropropane-d6	6.072	67	68453	5.478	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.600%
41) Toluene-d8	7.317	98	179276	4.311	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.200%
43) trans-1,3-Dichloroprop...	7.625	79	20550	4.893	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	97.800%
46) 2-Hexanone-d5	8.088	63	81815	55.500	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.000%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42688	5.407	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	63312	5.542	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.976	164	80746	8.491	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025665.D
Acq On : 21 Apr 2022 14:37
Operator : SY/MD
Sample : N2492-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T7


Quant Time: Apr 22 03:08:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 22 03:06:52 2022
Response via : Initial Calibration

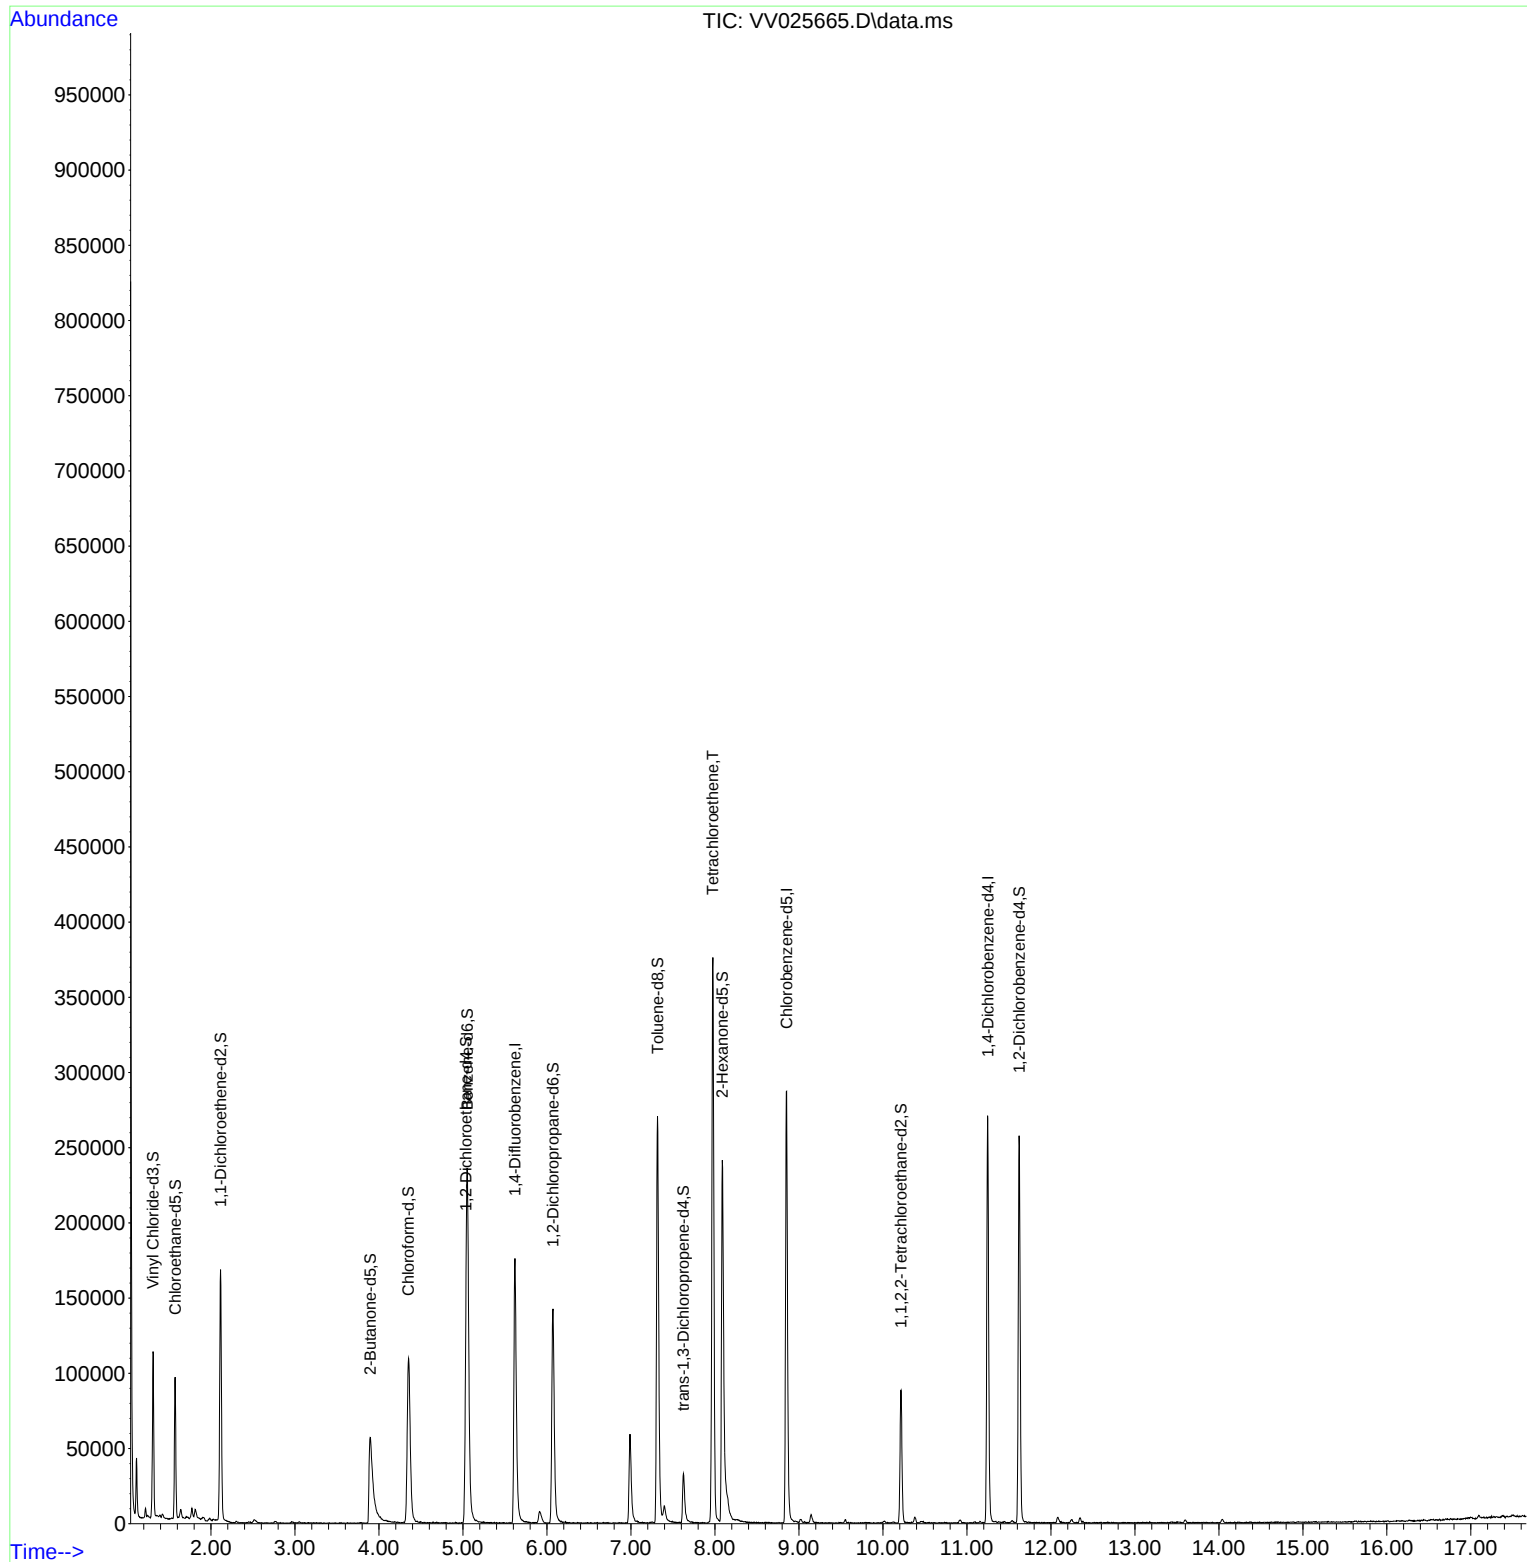

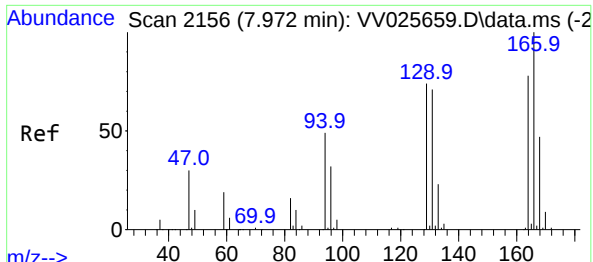

#47
 Tetrachloroethene
 Concen: 8.491 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV025665.D
 Acq: 21 Apr 2022 14:37

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T7

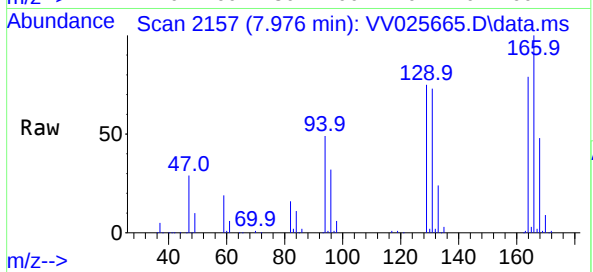

Tgt Ion:164 Resp: 80746

Ion	Ratio	Lower	Upper
164	100		
129	94.1	66.8	124.2
131	92.1	66.4	123.4
166	125.8	91.7	170.3

