

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042122\
 Data File : VW025670.D
 Acq On : 21 Apr 2022 16:34
 Operator : SY/MD
 Sample : N2492-08DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W0DL

Quant Time: Apr 22 03:10:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 22 03:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	111459	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	113772	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48619	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	42344	4.086	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.800%	
7) Chloroethane-d5	1.571	69	46227	4.193	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	83.800%	
11) 1,1-Dichloroethene-d2	2.111	63	67902	3.271	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.400%	
20) 2-Butanone-d5	3.902	46	92544	73.419	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	146.840%#	
24) Chloroform-d	4.352	84	87342	5.578	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	111.600%	
26) 1,2-Dichloroethane-d4	5.034	65	42891	6.357	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	127.200%	
32) Benzene-d6	5.053	84	163291	4.960	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
36) 1,2-Dichloropropane-d6	6.069	67	52772	5.748	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.000%	
41) Toluene-d8	7.317	98	130076	4.258	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.625	79	13986	4.532	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.088	63	60654	56.006	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	112.020%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	33091	5.705	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	114.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	46304	5.680	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds						
					Qvalue	
16) Methylene chloride	2.513	84	3568	0.381	ug/L	94
47) Tetrachloroethene	7.976	164	26803	3.837	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025670.D
Acq On : 21 Apr 2022 16:34
Operator : SY/MD
Sample : N2492-08DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Quant Time: Apr 22 03:10:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 22 03:06:52 2022
Response via : Initial Calibration




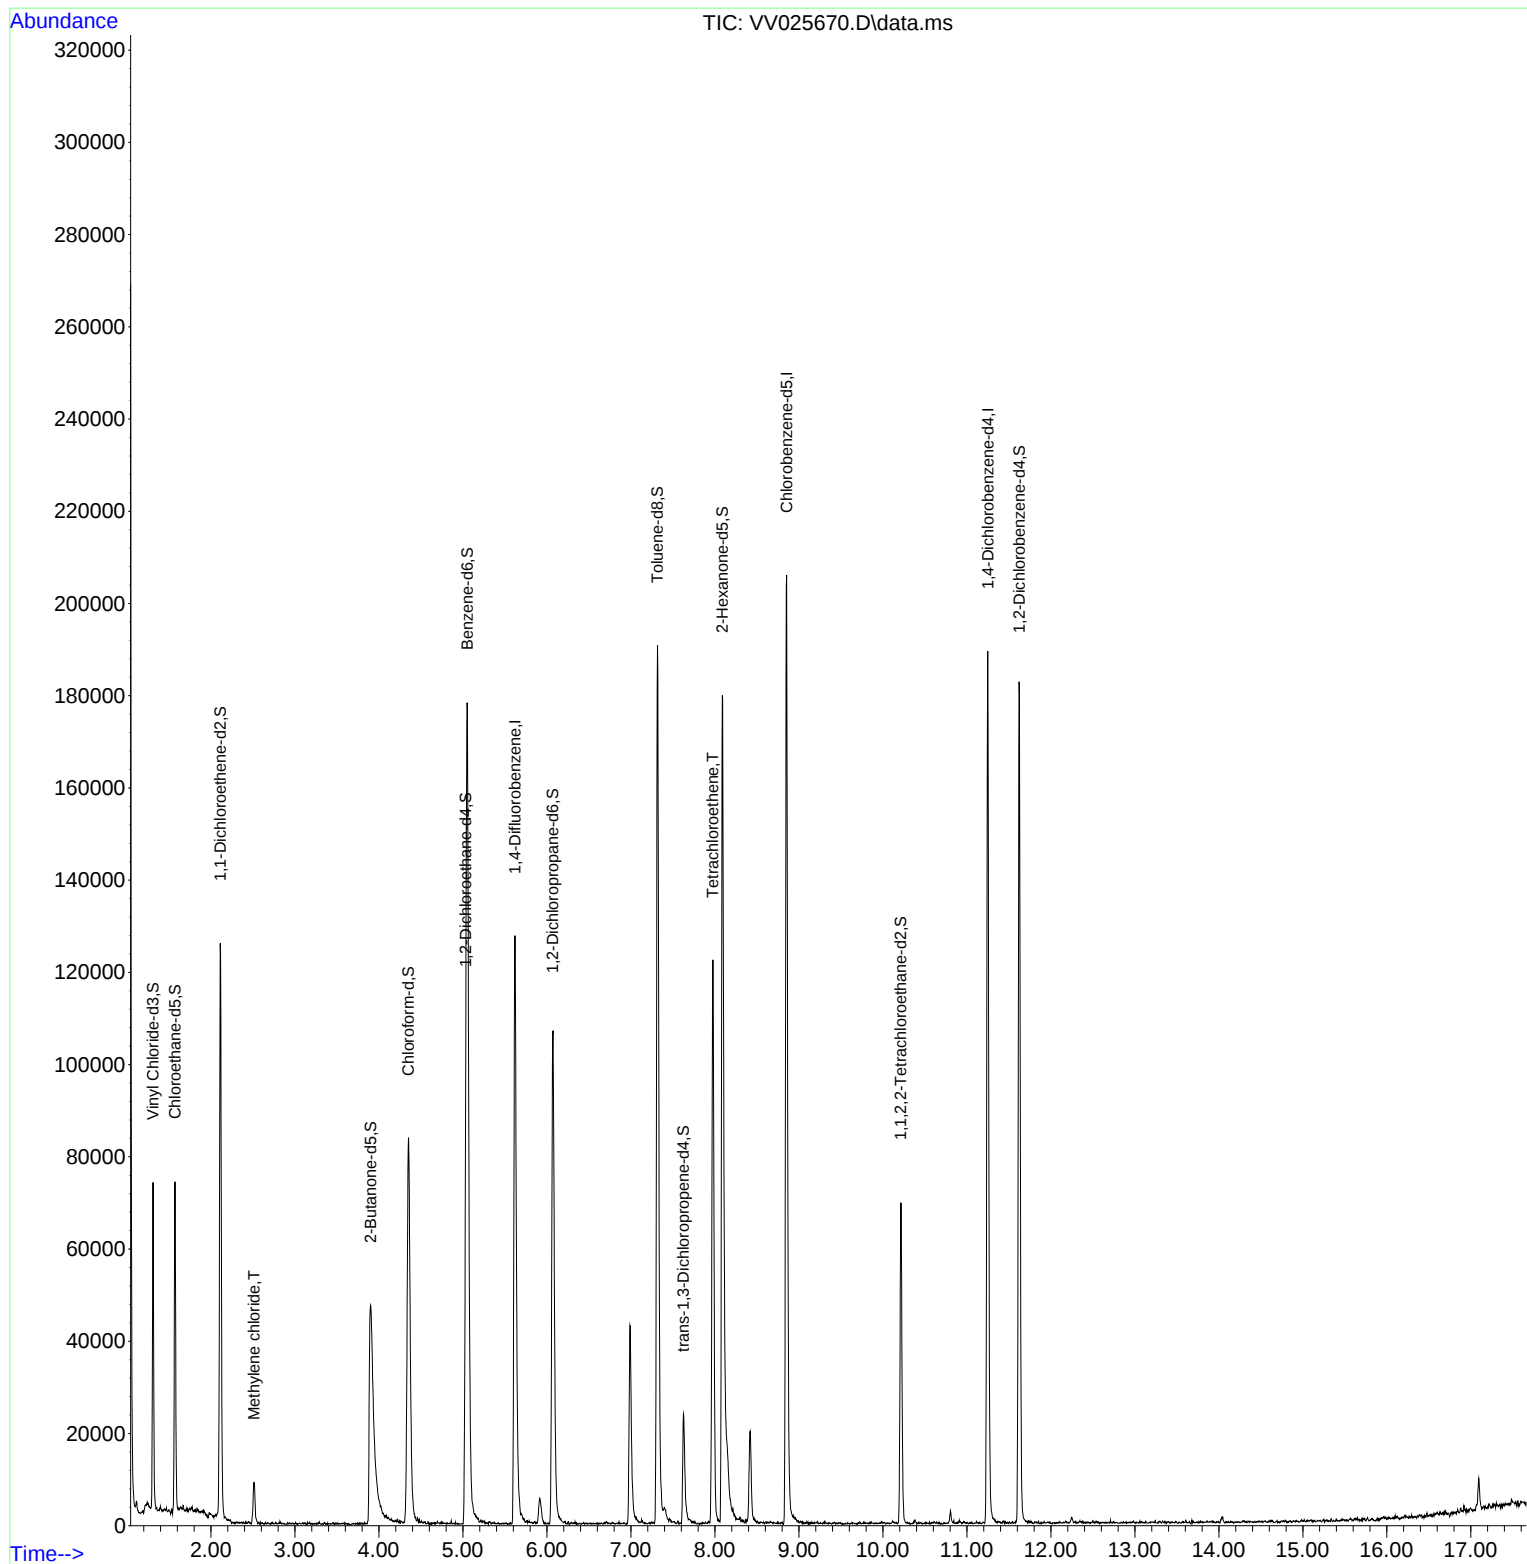


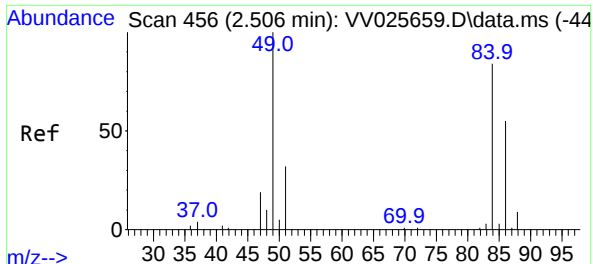

#16
Methylene chloride
Concen: 0.381 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV025670.D
Acq: 21 Apr 2022 16:34

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Tgt Ion: 84 Resp: 3568
Ion Ratio Lower Upper
84 100
86 62.5 45.9 85.3
49 116.3 76.6 142.3

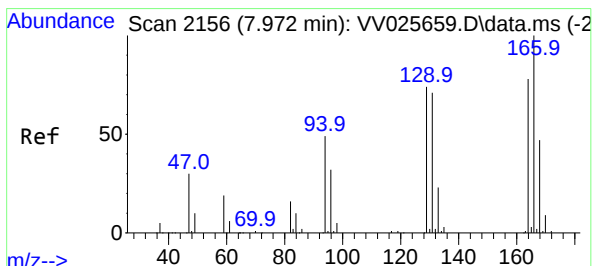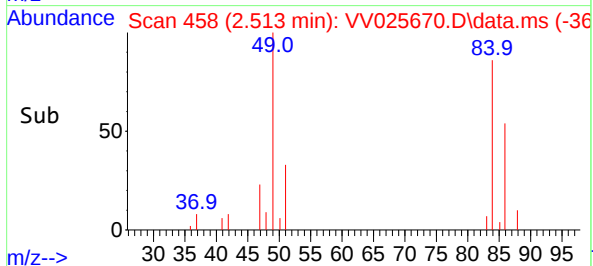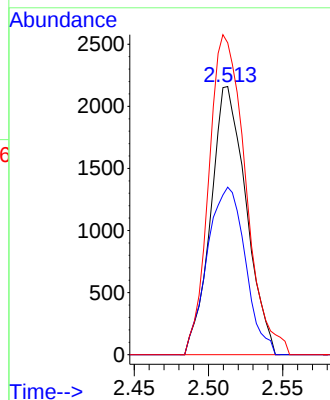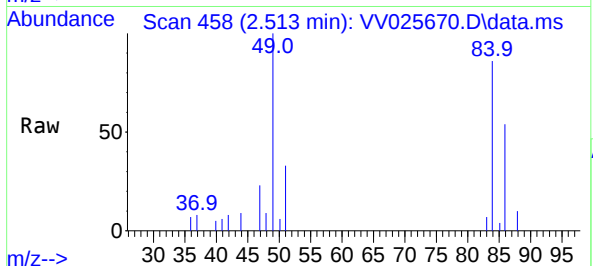

#47
Tetrachloroethene
Concen: 3.837 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. 0.003 min
Lab File: VV025670.D
Acq: 21 Apr 2022 16:34

Tgt Ion:164 Resp: 26803
Ion Ratio Lower Upper
164 100
129 100.3 66.8 124.2
131 97.1 66.4 123.4
166 129.4 91.7 170.3

