

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042122\
 Data File : VW025674.D
 Acq On : 21 Apr 2022 18:07
 Operator : SY/MD
 Sample : N2517-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH8

Quant Time: Apr 22 03:11:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 22 03:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	131163	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	135283	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	60928	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	43271	3.548	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.000%	
7) Chloroethane-d5	1.571	69	45214	3.485	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	69.800%	
11) 1,1-Dichloroethene-d2	2.111	63	69765	2.856	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	57.200%#	
20) 2-Butanone-d5	3.899	46	85203	57.441	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	114.880%	
24) Chloroform-d	4.352	84	90035	4.886	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.037	65	42324	5.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	5.053	84	163973	4.189	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.800%	
36) 1,2-Dichloropropane-d6	6.072	67	51932	4.757	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.200%	
41) Toluene-d8	7.317	98	134784	3.711	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.200%	
43) trans-1,3-Dichloroprop...	7.628	79	14611	3.982	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	79.600%	
46) 2-Hexanone-d5	8.088	63	58296	45.270	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.540%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31754	4.604	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	48056	4.704	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.000%	
Target Compounds						Qvalue
13) Acetone	2.182	43	4676	4.644	ug/L	56
25) Chloroform	4.384	83	8538	0.501	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025674.D
Acq On : 21 Apr 2022 18:07
Operator : SY/MD
Sample : N2517-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH8

Quant Time: Apr 22 03:11:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 22 03:06:52 2022
Response via : Initial Calibration




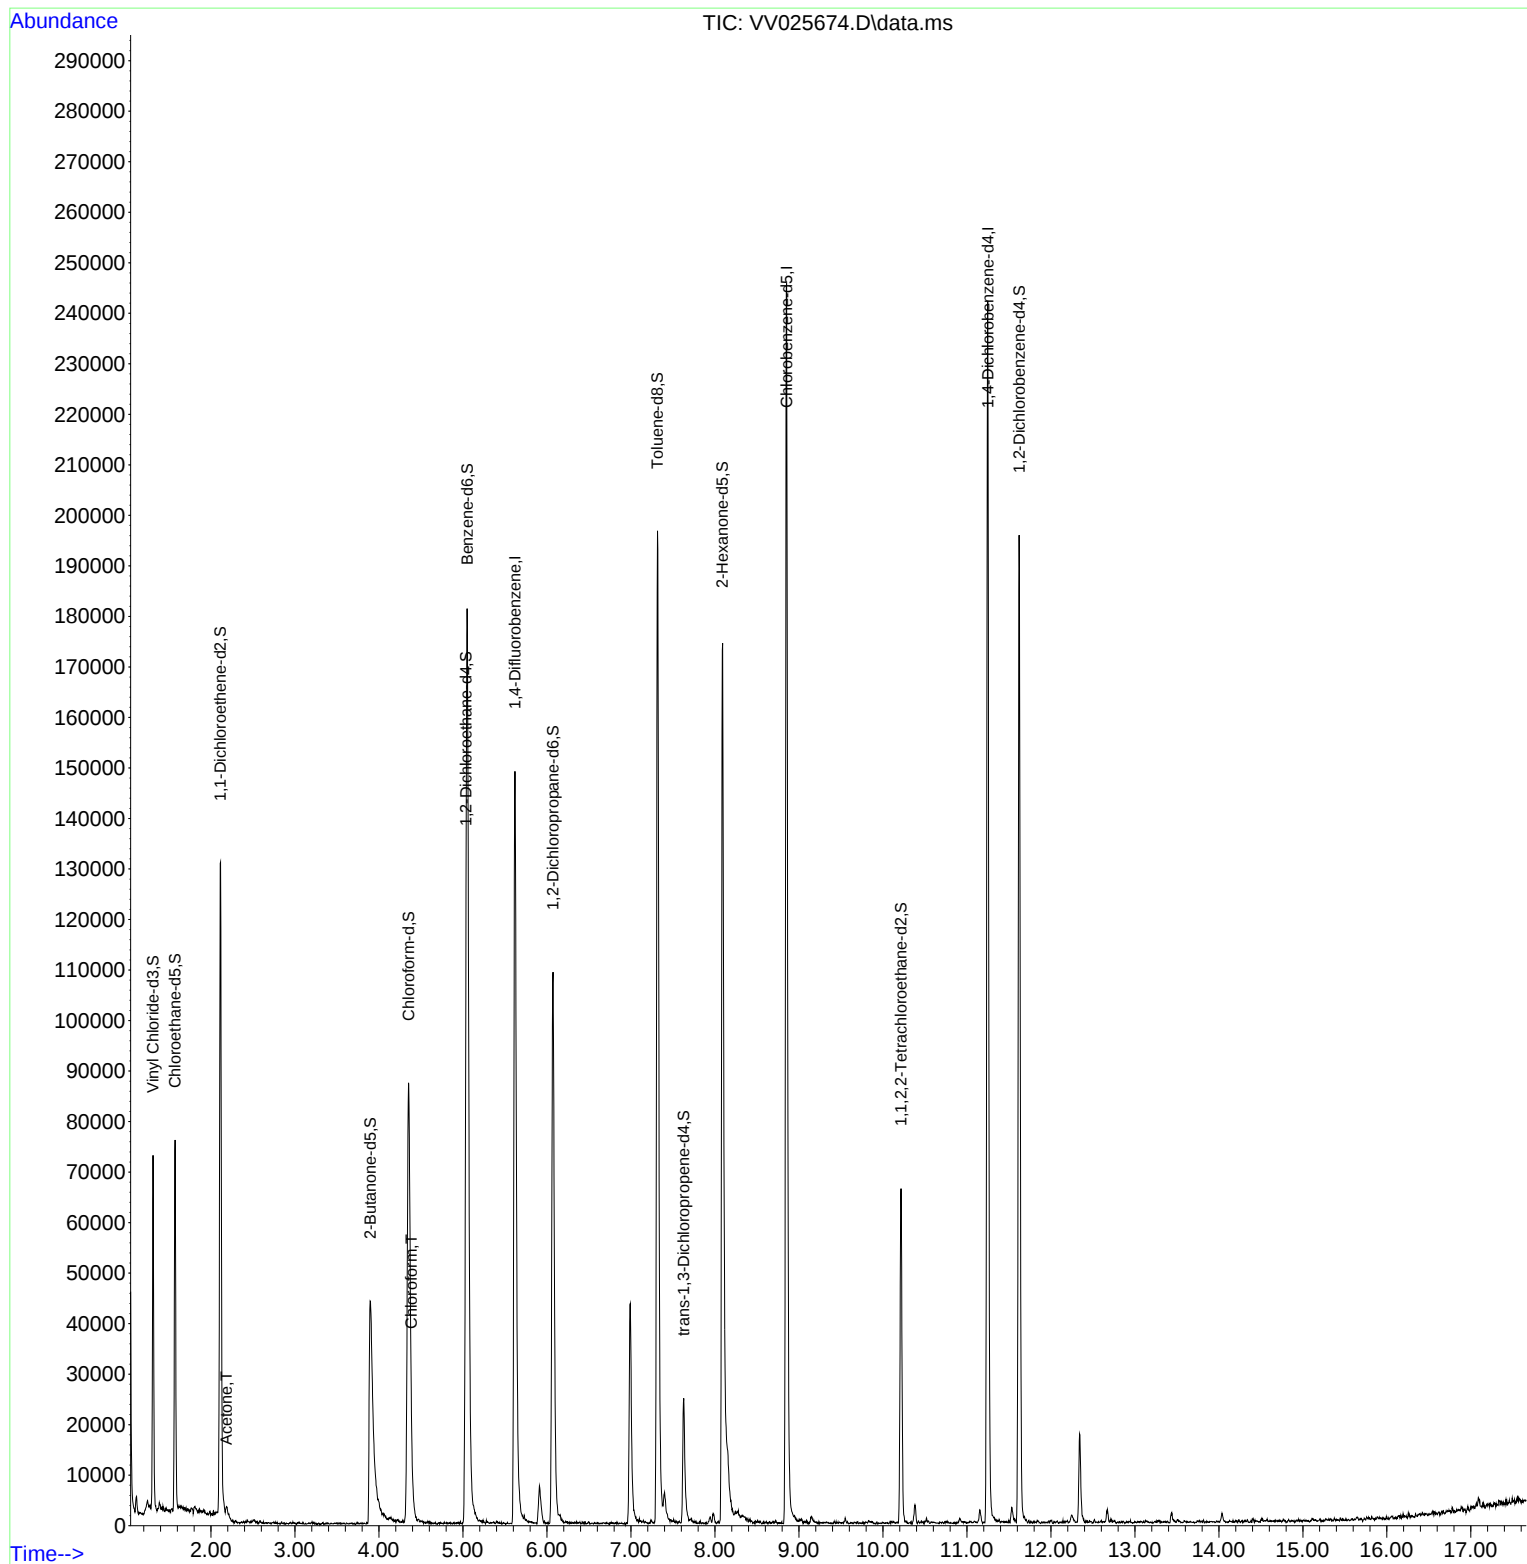


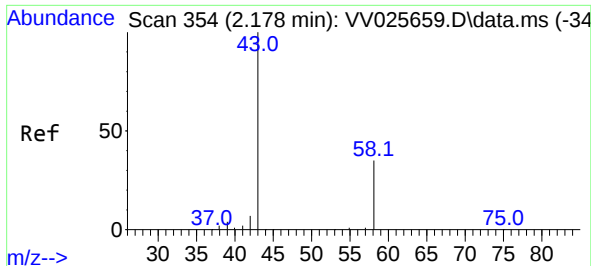

#13
Acetone
Concen: 4.644 ug/L
RT: 2.182 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV025674.D
Acq: 21 Apr 2022 18:07

Instrument :
MSVOA_V
ClientSampleId :
BFFH8

Tgt Ion: 43 Resp: 4676
Ion Ratio Lower Upper
43 100
58 10.2 0.0 72.2

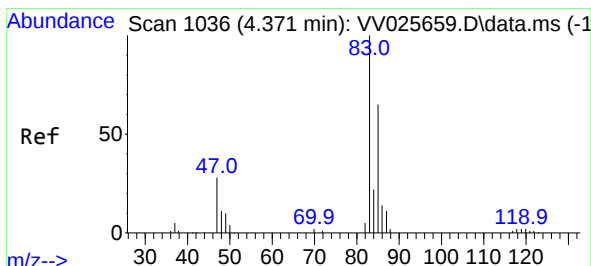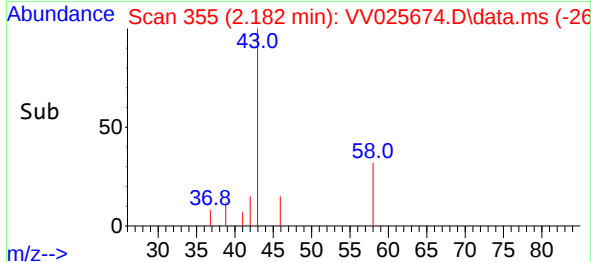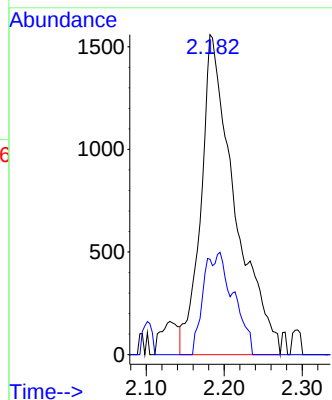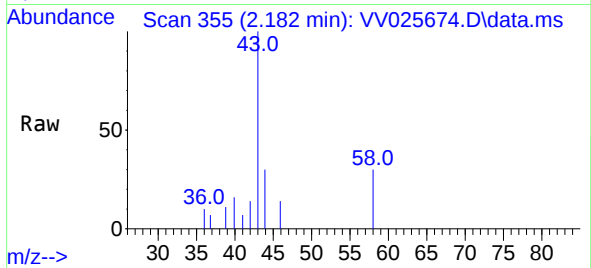

#25
Chloroform
Concen: 0.501 ug/L
RT: 4.384 min Scan# 1040
Delta R.T. 0.013 min
Lab File: VV025674.D
Acq: 21 Apr 2022 18:07

Tgt Ion: 83 Resp: 8538
Ion Ratio Lower Upper
83 100
85 64.4 43.5 80.7

