

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042122\
 Data File : VW025676.D
 Acq On : 21 Apr 2022 18:54
 Operator : SY/MD
 Sample : N2517-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH1

Quant Time: Apr 22 03:11:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Apr 22 03:06:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	135369	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	139197	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62790	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	40745	3.237	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.800%
7) Chloroethane-d5	1.571	69	43472	3.247	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	65.000%
11) 1,1-Dichloroethene-d2	2.111	63	64602	2.562	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.200%#
20) 2-Butanone-d5	3.899	46	72889	47.612	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.220%
24) Chloroform-d	4.352	84	86616	4.554	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	5.037	65	40189	4.904	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.000%
32) Benzene-d6	5.053	84	156520	3.886	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.800%
36) 1,2-Dichloropropane-d6	6.069	67	50419	4.489	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.800%
41) Toluene-d8	7.317	98	129452	3.464	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.200%#
43) trans-1,3-Dichloroprop...	7.628	79	13871	3.674	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.400%
46) 2-Hexanone-d5	8.088	63	55114	41.595	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	30844	4.347	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	45972	4.367	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.400%
Target Compounds						
13) Acetone	2.182	43	4146	3.990	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025676.D
Acq On : 21 Apr 2022 18:54
Operator : SY/MD
Sample : N2517-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH1

Quant Time: Apr 22 03:11:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Apr 22 03:06:52 2022
Response via : Initial Calibration

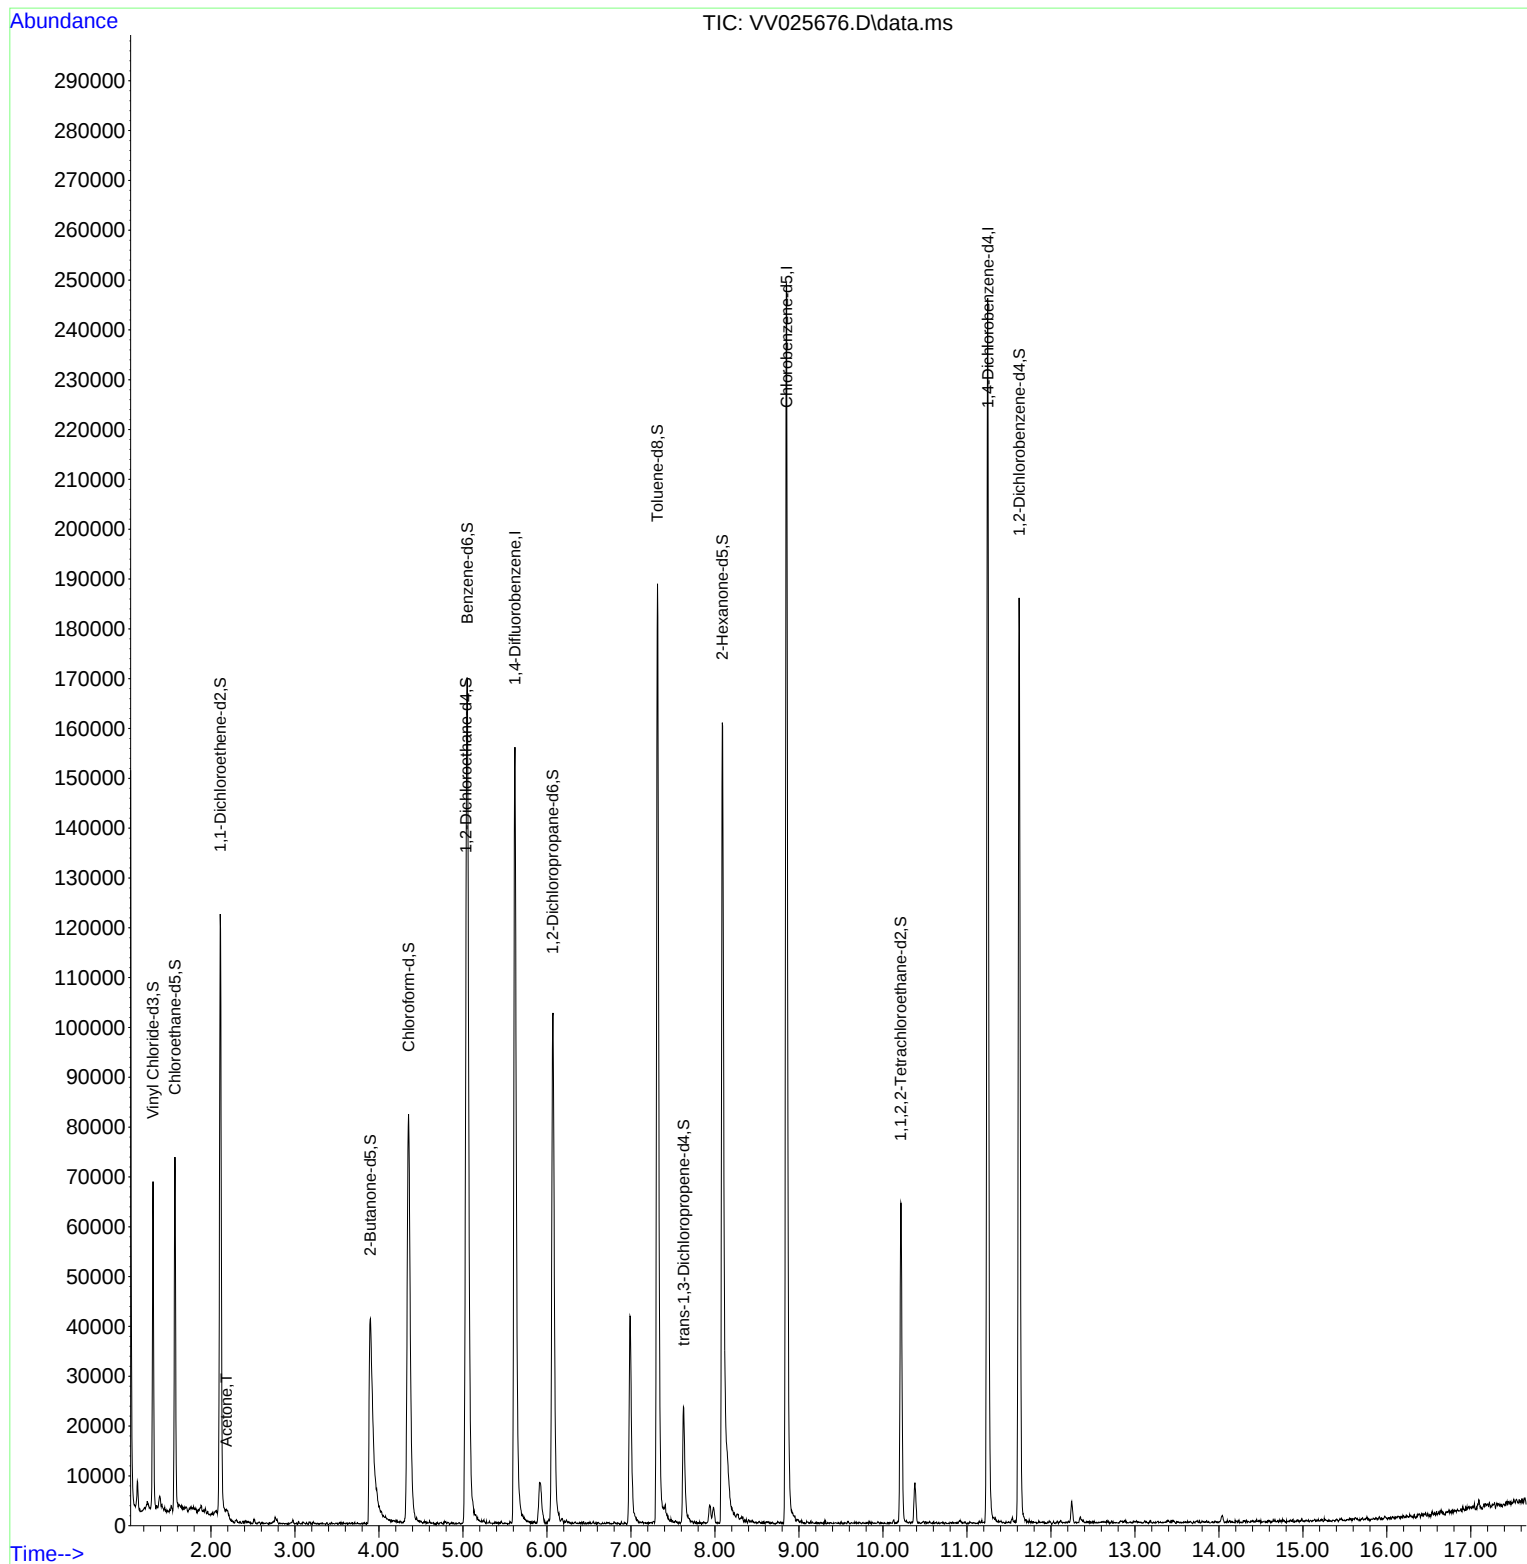

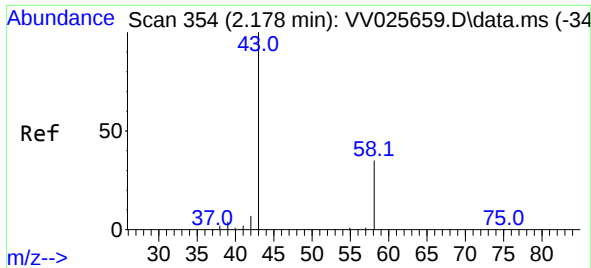

#13

Acetone

Concen: 3.990 ug/L

RT: 2.182 min Scan# 3

Delta R.T. 0.003 min

Lab File: VV025676.D


Acq: 21 Apr 2022 18:54

Instrument :

MSVOA_V

ClientSampleId :

BFFH1

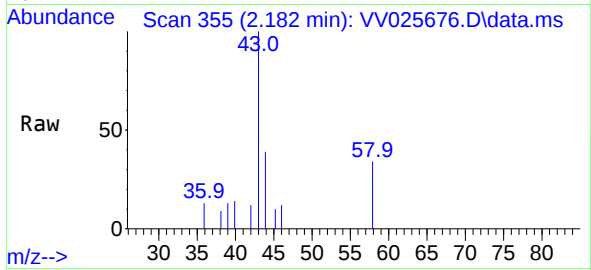

Tgt Ion: 43 Resp: 4146

Ion Ratio Lower Upper

43 100

58 31.9 0.0 72.2

