

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
 Data File : VV025663.D
 Acq On : 21 Apr 2022 13:50
 Operator : SY/MD
 Sample : N2492-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.114	17	23	30	rVB3	7776	8172	1.20%	0.153%
2	1.310	76	84	95	rBV	111345	114061	16.71%	2.134%
3	1.571	158	165	179	rBV	105838	122181	17.90%	2.286%
4	2.114	323	334	351	rVB	199101	291931	42.78%	5.463%
5	2.516	450	459	471	rBV2	9945	17433	2.55%	0.326%
6	3.905	880	891	893	rBV	47724	69106	10.13%	1.293%
7	4.352	1013	1030	1058	rBV2	132138	380641	55.78%	7.122%
8	5.050	1226	1247	1280	rBV3	268356	682430	100.00%	12.769%
9	5.619	1413	1424	1451	rBV	178077	364435	53.40%	6.819%
10	5.915	1505	1516	1531	rBV4	8561	19570	2.87%	0.366%
11	6.072	1552	1565	1583	rBV	160601	329887	48.34%	6.173%
12	6.516	1692	1703	1719	rBV6	5004	10626	1.56%	0.199%
13	6.989	1839	1850	1871	rBV2	67170	128712	18.86%	2.408%
14	7.317	1937	1952	1971	rBV	324238	560095	82.07%	10.480%
15	7.625	2039	2048	2070	rBV	38398	71099	10.42%	1.330%
16	7.940	2135	2146	2154	rBV4	4699	8928	1.31%	0.167%
17	8.092	2182	2193	2226	rBV	262054	552552	80.97%	10.339%
18	8.854	2419	2430	2458	rBV	289516	479957	70.33%	8.981%
19	10.214	2840	2853	2873	rBV	100918	159249	23.34%	2.980%
20	10.381	2891	2905	2918	rVB2	13916	22280	3.26%	0.417%
21	11.246	3163	3174	3198	rBV	270287	426062	62.43%	7.972%
22	11.532	3254	3263	3278	rBV2	9435	16017	2.35%	0.300%
23	11.622	3278	3291	3312	rVB	301251	465531	68.22%	8.711%
24	12.249	3474	3486	3496	rBV2	8871	13923	2.04%	0.261%
25	12.345	3507	3516	3531	rBV2	13315	20710	3.03%	0.388%
26	13.432	3844	3854	3863	rBV5	6217	8643	1.27%	0.162%




Sum of corrected areas: 5344231

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025663.D
Acq On : 21 Apr 2022 13:50
Operator : SY/MD
Sample : N2492-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

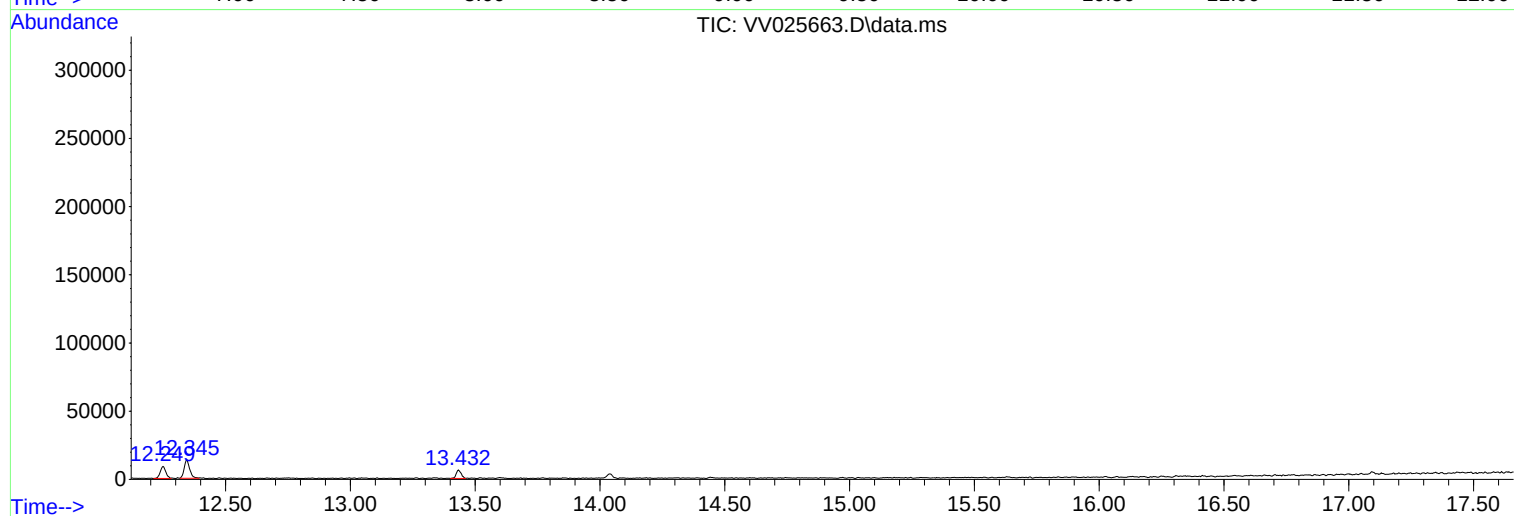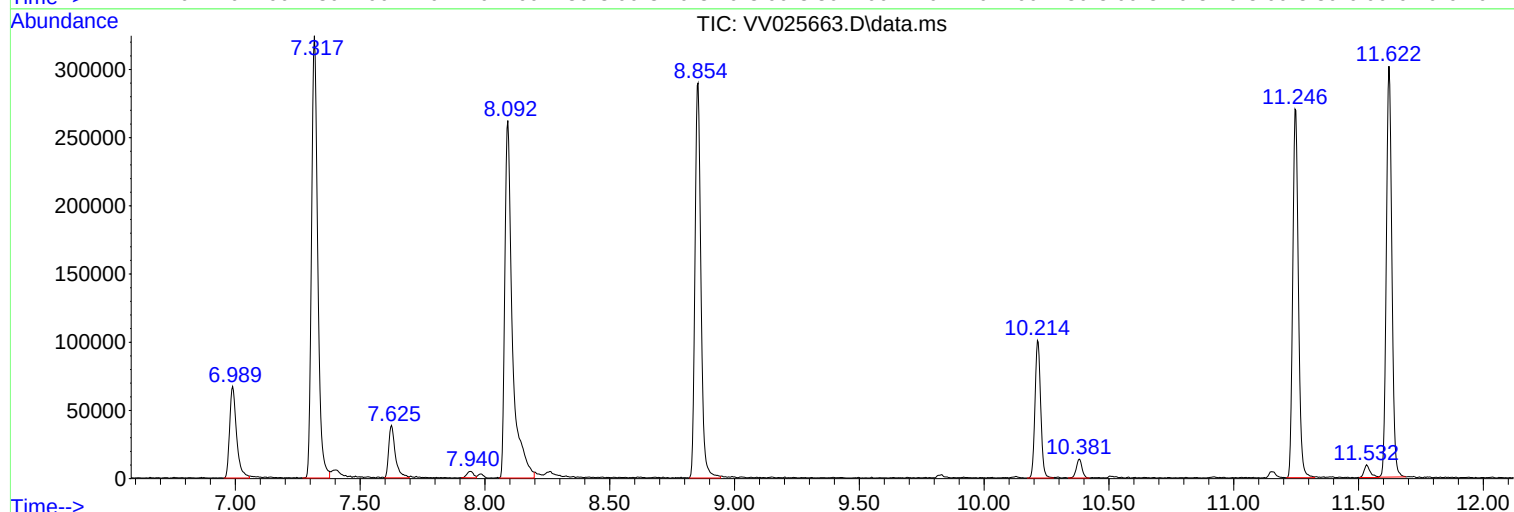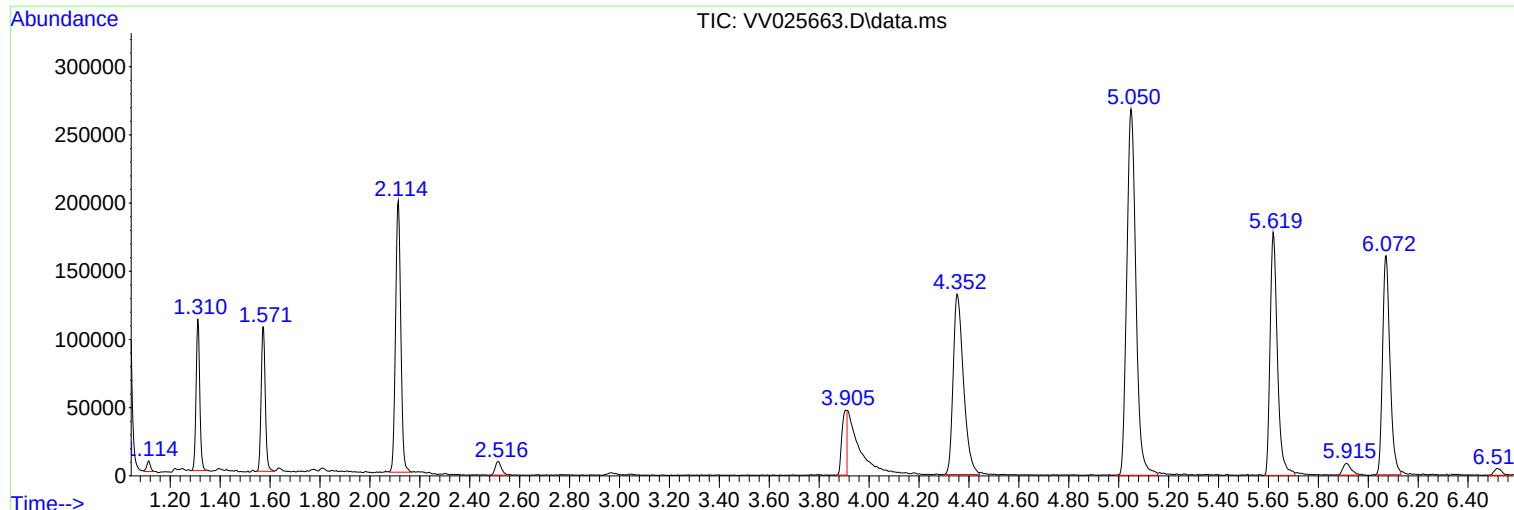

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025663.D
Acq On : 21 Apr 2022 13:50
Operator : SY/MD
Sample : N2492-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025663.D
Acq On : 21 Apr 2022 13:50
Operator : SY/MD
Sample : N2492-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------