

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
 Data File : VV025672.D
 Acq On : 21 Apr 2022 17:21
 Operator : SY/MD
 Sample : N2492-04DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	78	84	93	rVB	66510	65566	13.84%	1.717%
2	1.571	158	165	177	rBV	73478	85671	18.08%	2.244%
3	2.114	320	334	353	rVB	118572	177947	37.55%	4.660%
4	2.513	448	458	473	rVB3	7852	13949	2.94%	0.365%
5	3.899	875	889	925	rBV3	55447	201176	42.46%	5.269%
6	4.352	1015	1030	1062	rBV3	87959	226708	47.84%	5.937%
7	5.050	1230	1247	1278	rBV2	186745	473841	100.00%	12.410%
8	5.619	1409	1424	1444	rBV	127604	263998	55.71%	6.914%
9	5.915	1506	1516	1532	rBV6	7037	15375	3.24%	0.403%
10	6.072	1551	1565	1588	rBV	114659	237698	50.16%	6.225%
11	6.989	1840	1850	1872	rBV	46929	87211	18.41%	2.284%
12	7.317	1941	1952	1970	rBV	189798	334770	70.65%	8.767%
13	7.625	2038	2048	2070	rBV2	25521	49594	10.47%	1.299%
14	7.976	2146	2157	2172	rBV	68594	115778	24.43%	3.032%
15	8.088	2183	2192	2235	rBV	197007	413250	87.21%	10.823%
16	8.419	2284	2295	2311	rBV2	18805	33950	7.16%	0.889%
17	8.854	2417	2430	2446	rBV	200770	332116	70.09%	8.698%
18	10.217	2842	2854	2871	rBV	75045	119300	25.18%	3.124%
19	11.249	3164	3175	3198	rBV	179056	280382	59.17%	7.343%
20	11.622	3280	3291	3309	rBV	176945	283737	59.88%	7.431%
21	17.094	4985	4993	5003	rBV4	3718	6319	1.33%	0.165%




Sum of corrected areas: 3818336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025672.D
Acq On : 21 Apr 2022 17:21
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

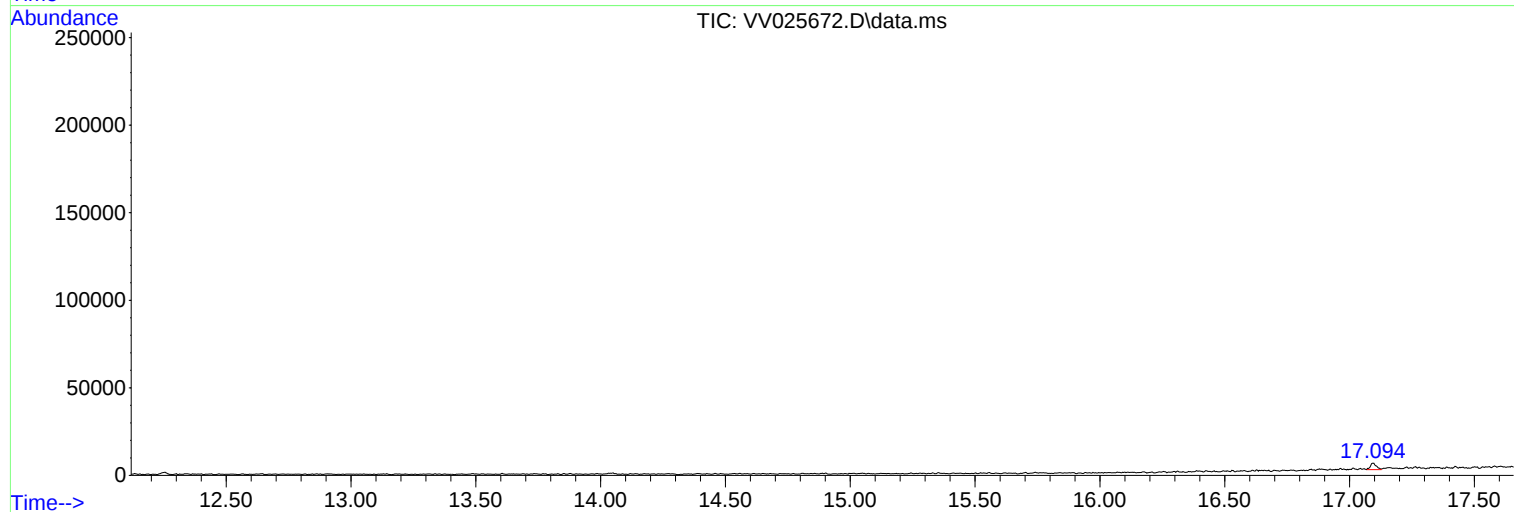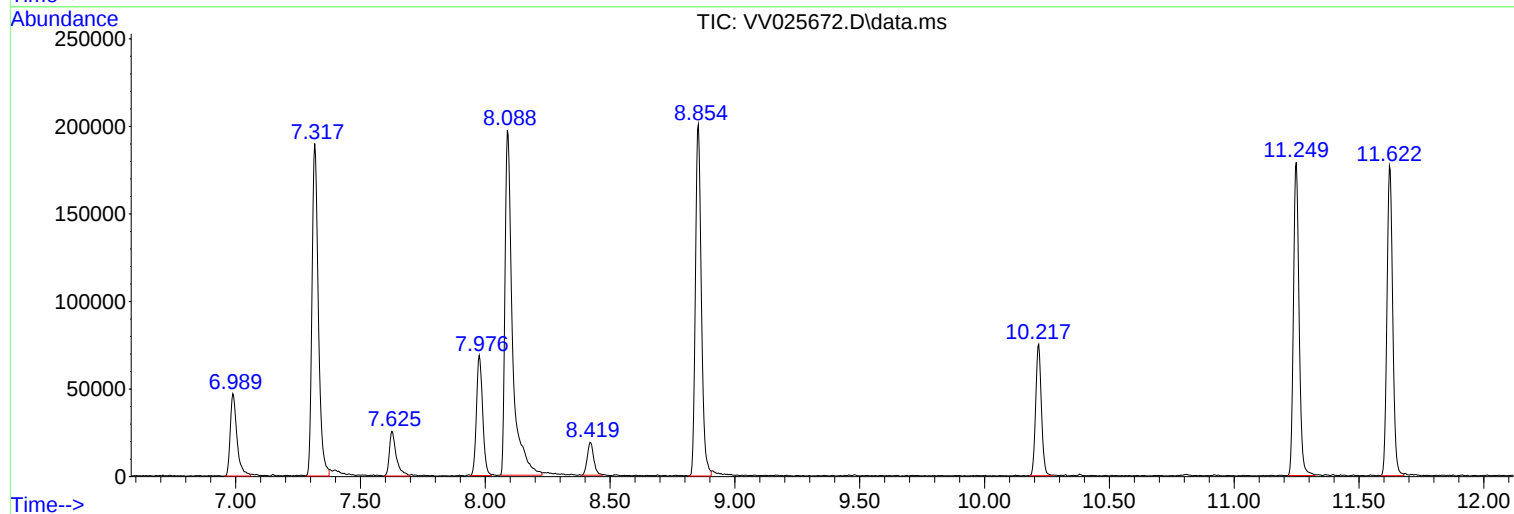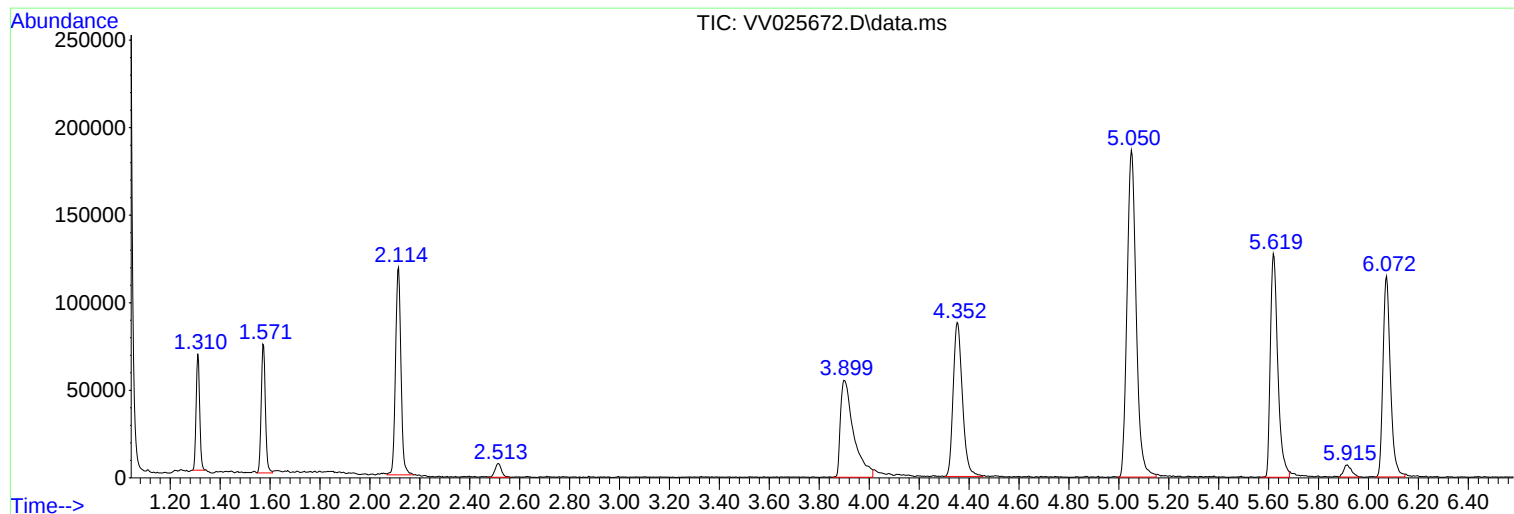

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025672.D
Acq On : 21 Apr 2022 17:21
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.419	0.51 ug/L	33950	Chlorobenzene-d5	8.854

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Indole-3-thiol	149	C8H7NS	000480-94-4	35
2			1,2,4-Triazole, 3,5-dithio-	133	C2H3N3S2	005650-03-3	30
3			4-Ethylbenzoic acid, 2,2-dimethy...	220	C14H20O2	1000293-49-5	17
4			Phosphonoselenic difluoride	150	F2HPSe	026144-62-7	16
5			Silane, diethoxydimethyl-	148	C6H16O2Si	000078-62-6	16

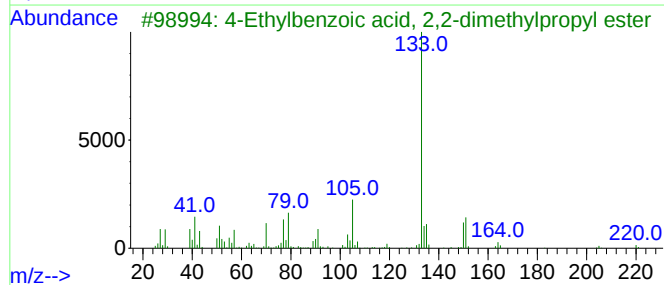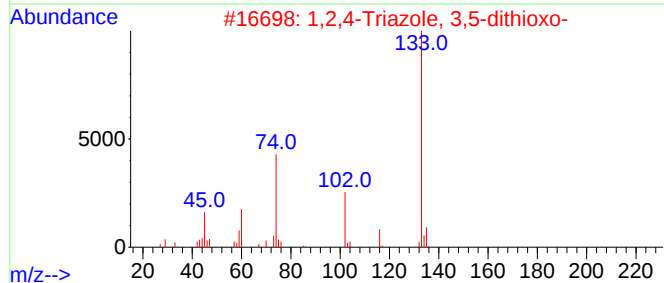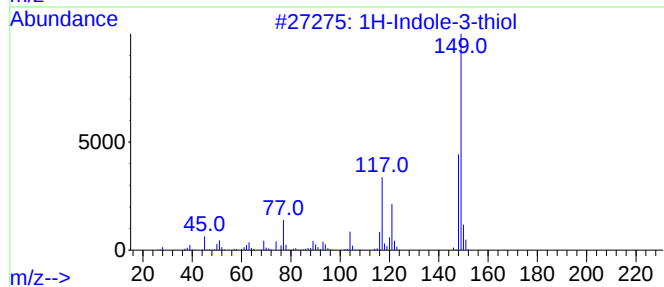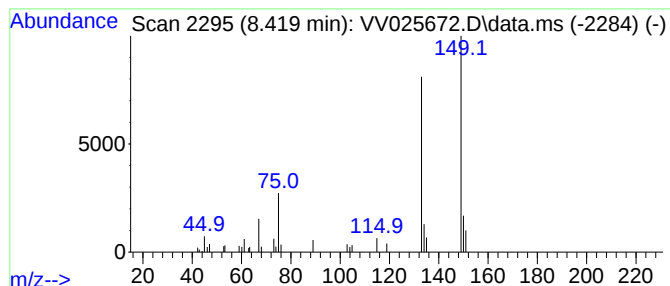

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025672.D
Acq On : 21 Apr 2022 17:21
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	8.419	0.5	ug/L	33950	2	8.854	332116	5.0