

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
 Data File : VV025676.D
 Acq On : 21 Apr 2022 18:54
 Operator : SY/MD
 Sample : N2517-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	33	rVB	5863	6395	1.48%	0.174%
2	1.310	76	84	95	rVB	65680	68032	15.70%	1.852%
3	1.571	157	165	174	rBV	71073	81114	18.72%	2.208%
4	2.111	323	333	347	rBV	120271	175452	40.50%	4.777%
5	3.899	879	889	911	rBV2	41148	128025	29.55%	3.485%
6	4.352	1015	1030	1057	rBV	81707	209457	48.35%	5.702%
7	5.050	1229	1247	1277	rBV3	169795	433234	100.00%	11.794%
8	5.619	1412	1424	1450	rBV	155749	318611	73.54%	8.674%
9	5.915	1505	1516	1533	rBV9	8156	20406	4.71%	0.556%
10	6.072	1552	1565	1586	rBV2	101857	213222	49.22%	5.805%
11	6.989	1838	1850	1865	rBV2	41845	79300	18.30%	2.159%
12	7.317	1941	1952	1972	rBV	188546	335361	77.41%	9.130%
13	7.625	2038	2048	2062	rBV	23214	42188	9.74%	1.149%
14	7.937	2134	2145	2152	rBV4	3677	6349	1.47%	0.173%
15	7.982	2153	2159	2169	rVB7	3145	5157	1.19%	0.140%
16	8.088	2181	2192	2226	rBV	160748	337052	77.80%	9.176%
17	8.850	2419	2429	2447	rBV	248864	418100	96.51%	11.382%
18	10.214	2843	2853	2869	rBV	64030	100783	23.26%	2.744%
19	10.381	2895	2905	2916	rVB3	8093	13132	3.03%	0.358%
20	11.249	3163	3175	3193	rBV	245845	379755	87.66%	10.339%
21	11.622	3279	3291	3313	rBV	185547	295764	68.27%	8.052%
22	12.249	3478	3486	3496	rVB	4384	6303	1.45%	0.172%


Sum of corrected areas: 3673192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025676.D
Acq On : 21 Apr 2022 18:54
Operator : SY/MD
Sample : N2517-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

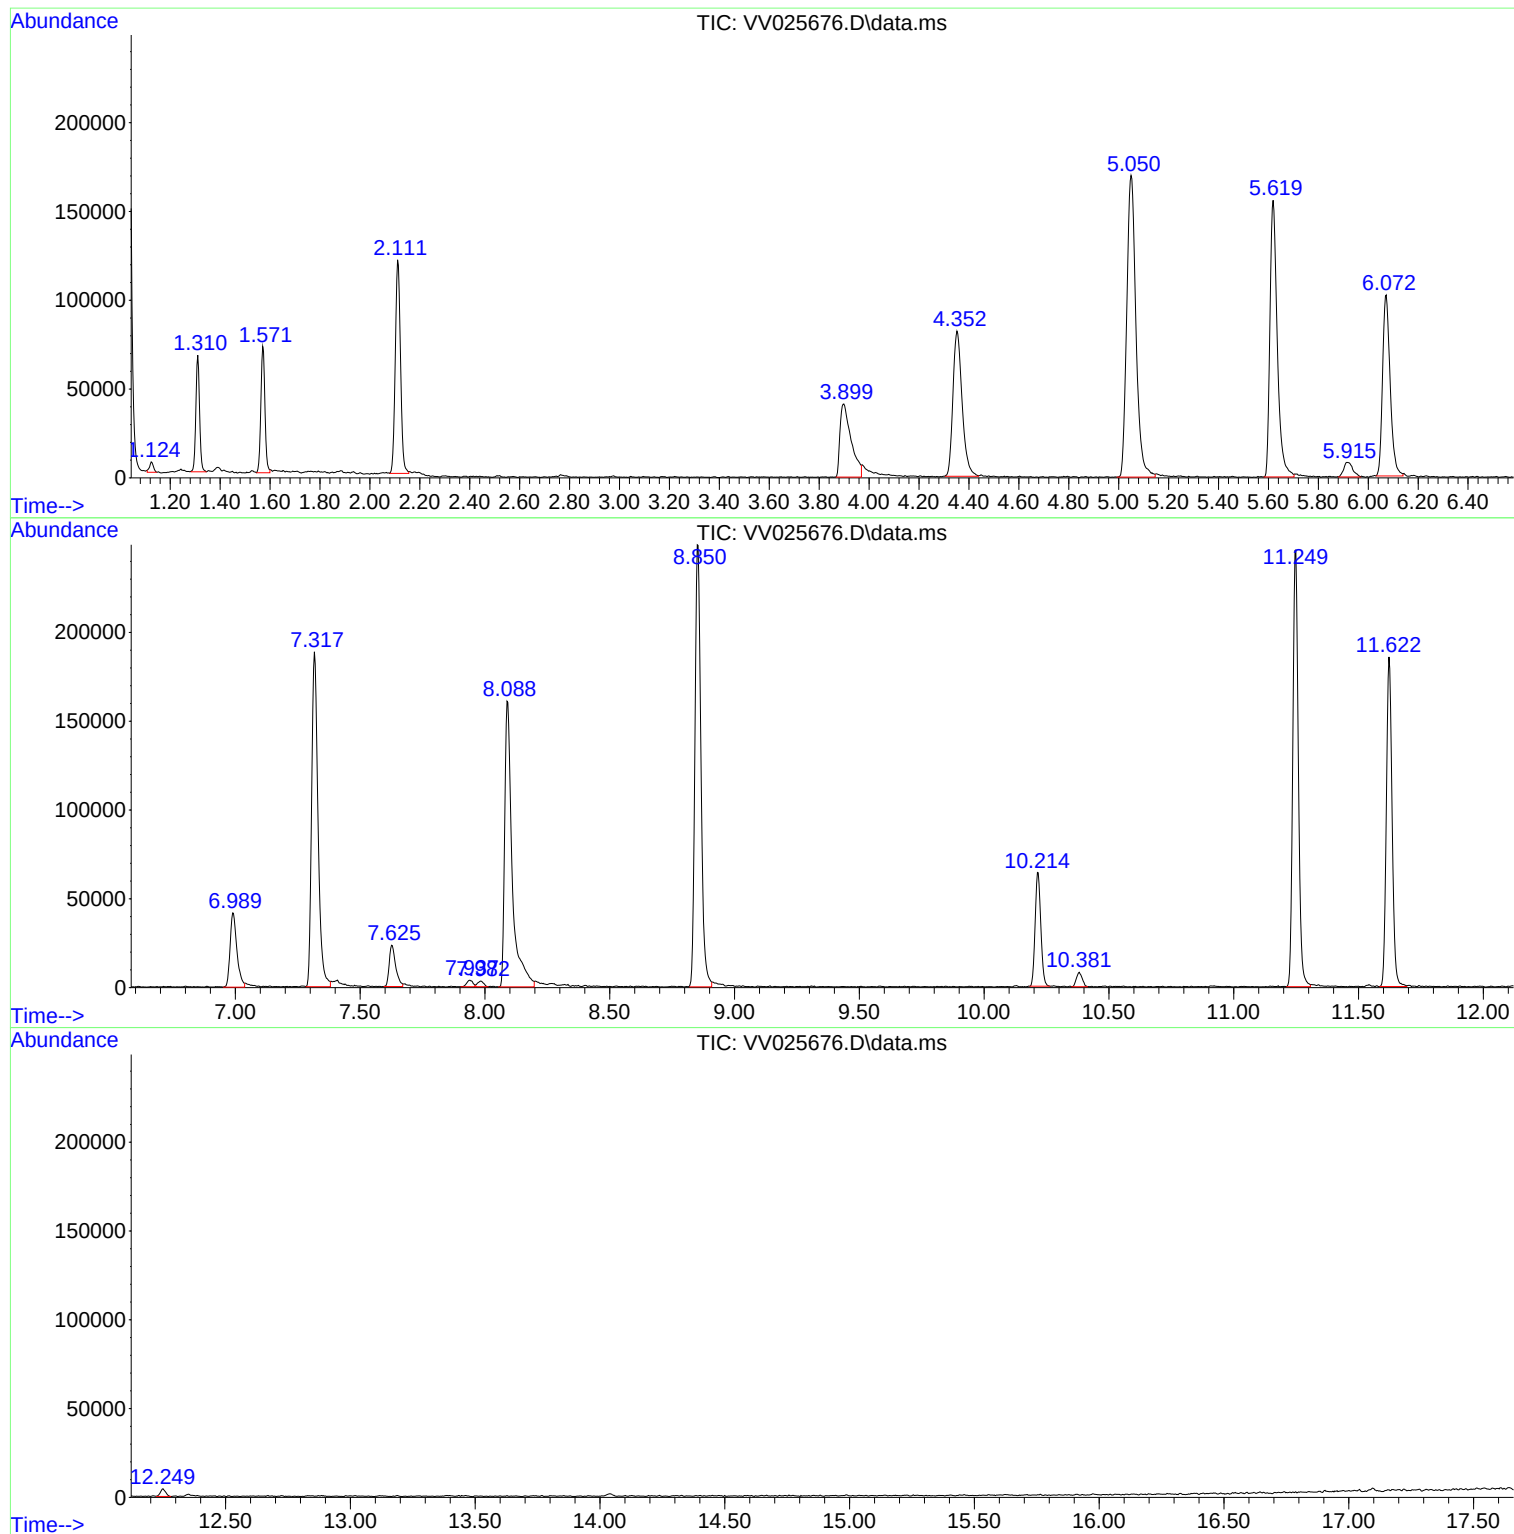

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025676.D
Acq On : 21 Apr 2022 18:54
Operator : SY/MD
Sample : N2517-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
Data File : VV025676.D
Acq On : 21 Apr 2022 18:54
Operator : SY/MD
Sample : N2517-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
