
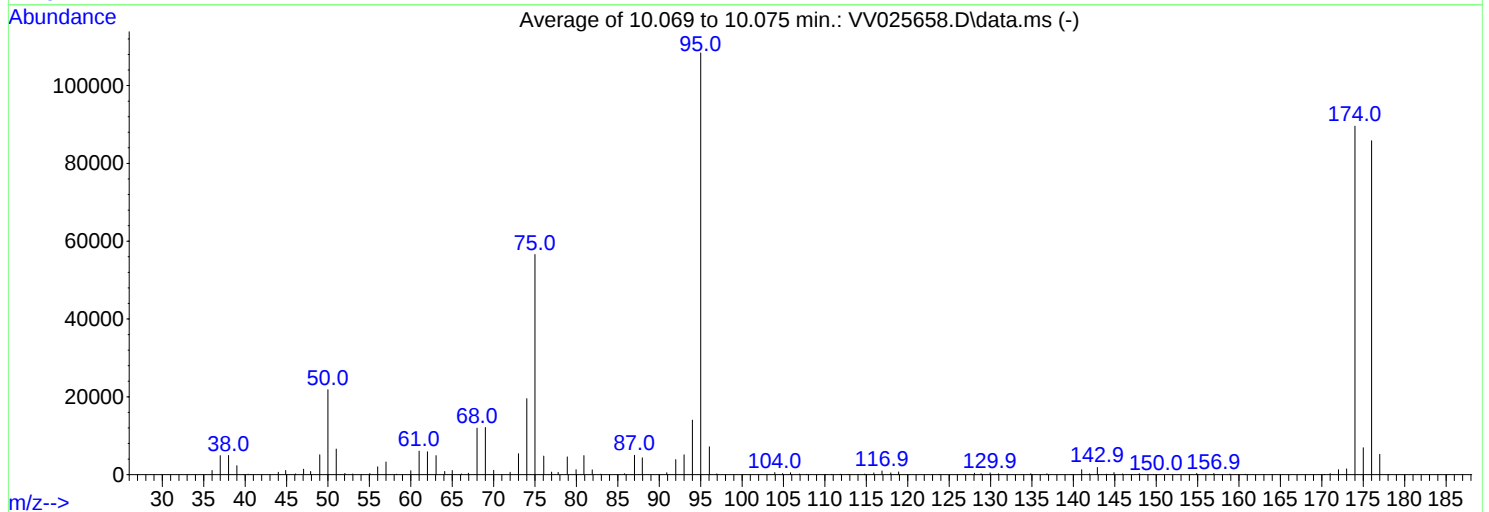


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042122\
 Data File : VV025658.D
 Acq On : 21 Apr 2022 09:37
 Operator : SY/MD
 Sample : BFB307
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB307

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Apr 26 06:32:17 2022

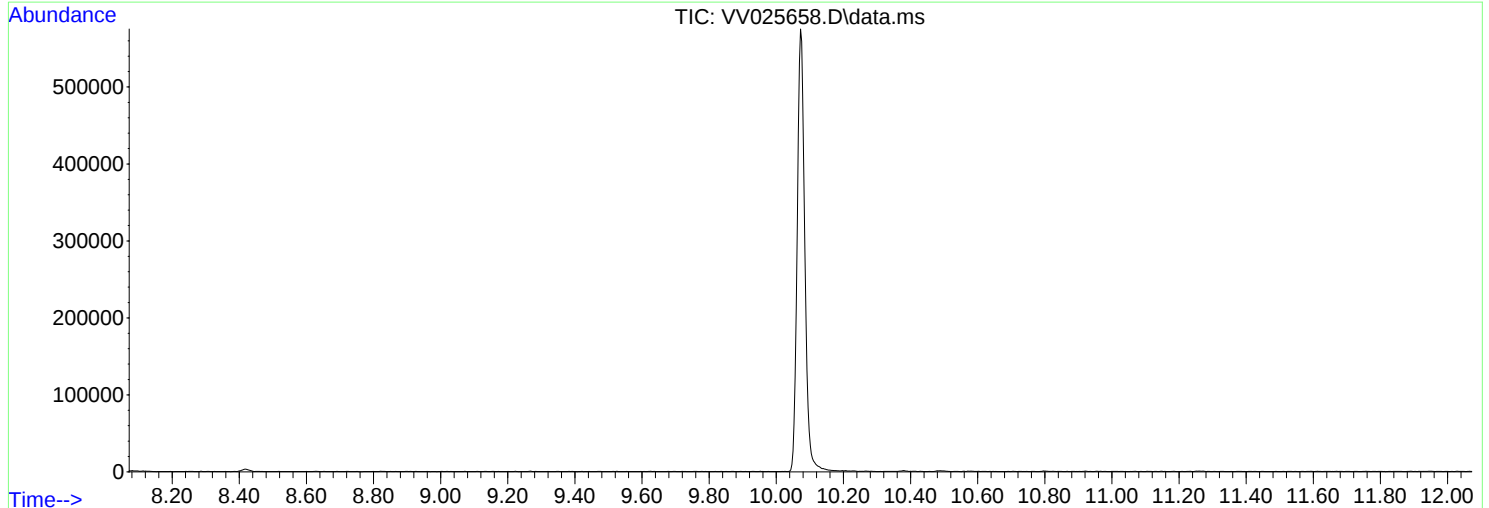

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	21832	PASS
75	95	30	80	52.2	56605	PASS
95	95	100	100	100.0	108413	PASS
96	95	5	9	6.6	7168	PASS
173	174	0.00	2	1.7	1486	PASS
174	95	50	120	82.6	89584	PASS
175	174	5	9	7.7	6914	PASS
176	174	95	105	95.8	85808	PASS
177	176	5	10	6.1	5243	PASS

m/z	Abundance
39.90	192.0
44.00	336.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	1016.0
37.00	4810.0
38.00	5081.0
39.00	2122.0
39.90	245.0
40.40	181.0
40.70	164.0
44.00	945.0
44.90	996.0
46.10	233.0
47.10	1397.0
47.90	767.0
49.00	5004.0
50.00	21304.0
51.00	6446.0
52.10	324.0
53.00	166.0
55.10	301.0
56.00	1949.0
57.00	3211.0
58.30	143.0
60.00	1004.0
61.00	5907.0
62.00	5782.0
63.10	4799.0
64.10	825.0
65.00	1105.0
66.20	143.0
67.00	363.0
68.00	11412.0
69.00	11549.0
70.00	1042.0
72.00	607.0
73.00	5369.0
74.00	18904.0
75.00	53648.0
76.00	4651.0
77.00	629.0
77.80	580.0
78.90	4404.0
79.90	1264.0
80.90	4722.0
81.90	1113.0
82.90	129.0
85.80	235.0
87.00	4890.0
88.00	4268.0
90.90	467.0
92.00	3719.0
93.00	5060.0
94.00	13247.0
95.00	103928.0
96.10	6931.0
96.90	247.0
104.00	523.0
104.90	296.0
105.90	515.0
107.00	132.0
110.10	117.0
110.80	135.0
111.90	143.0
112.80	129.0
114.80	175.0
115.90	414.0
116.90	1002.0
117.90	395.0
118.90	703.0
123.80	101.0
128.00	365.0
128.80	248.0
130.00	458.0
131.00	224.0
133.80	117.0
134.90	279.0
136.80	212.0
141.00	1177.0
141.90	200.0
142.90	1853.0
144.00	141.0
144.90	509.0
145.90	203.0
147.90	242.0
150.00	141.0
154.90	287.0
157.00	313.0
158.90	158.0
160.70	106.0
170.30	151.0
171.10	283.0
172.00	1206.0
173.00	1417.0
174.00	83888.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

175.00	6698.0
176.00	80880.0
177.00	5123.0
178.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	1098.0
37.00	4963.0
38.00	5070.0
39.00	2375.0
39.80	242.0
40.30	197.0
44.00	968.0
44.90	1106.0
46.10	196.0
47.00	1479.0
47.90	899.0
49.00	5354.0
50.00	22688.0
51.00	6821.0
52.00	354.0
53.00	161.0
55.00	278.0
56.00	2079.0
57.00	3400.0
58.30	142.0
60.00	1069.0
61.00	6281.0
62.00	6122.0
63.10	5022.0
64.10	870.0
65.00	1086.0
66.10	161.0
67.00	376.0
68.00	12494.0
69.00	12609.0
70.00	1138.0
72.00	664.0
73.00	5618.0
74.00	20112.0
75.00	58768.0
76.10	4867.0
77.00	701.0
77.80	633.0
78.90	4650.0
80.00	1312.0
80.90	5061.0
81.90	1282.0
83.00	121.0
85.80	262.0
87.00	5079.0
88.00	4377.0
90.90	531.0
92.00	4017.0
93.00	5270.0
94.00	14583.0
95.00	112224.0
96.10	7425.0
96.90	201.0
104.00	533.0
104.90	300.0
105.90	509.0
107.00	155.0
107.80	101.0
110.10	123.0
110.80	105.0
111.80	156.0
112.80	115.0
114.80	170.0
115.90	489.0
116.90	1010.0
118.00	482.0
118.90	700.0
128.00	388.0
128.90	235.0
130.00	501.0
131.00	261.0
134.90	284.0
136.80	254.0
141.00	1332.0
141.90	227.0
142.90	1942.0
144.00	143.0
144.90	571.0
145.90	219.0
148.00	290.0
149.70	110.0
150.00	109.0
154.90	342.0
156.90	335.0
158.90	171.0
160.70	114.0
170.30	141.0
171.00	281.0
172.00	1325.0
173.00	1578.0
174.00	92776.0
175.00	7208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

176.0088832.0

177.005417.0

178.10107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307

m/z	Abundance
36.00	1042.0
37.00	4870.0
38.00	4643.0
39.00	2367.0
39.80	251.0
44.00	977.0
44.90	1092.0
46.10	149.0
47.00	1322.0
47.90	856.0
49.00	5000.0
50.00	21504.0
51.00	6496.0
52.00	315.0
52.90	155.0
54.10	128.0
55.00	283.0
56.00	2013.0
57.00	3102.0
58.30	120.0
60.00	1034.0
61.00	5952.0
62.00	5803.0
63.00	4873.0
64.10	815.0
65.00	979.0
66.00	163.0
66.90	331.0
68.00	11954.0
69.00	12249.0
70.00	1134.0
72.00	627.0
73.00	5189.0
74.00	19552.0
75.00	57400.0
76.10	4750.0
77.00	671.0
77.80	541.0
78.90	4590.0
80.00	1258.0
80.90	4898.0
81.90	1293.0
83.00	128.0
85.80	217.0
87.00	4961.0
87.90	4331.0
90.90	516.0
92.00	3885.0
93.00	5014.0
94.00	14257.0
95.00	109088.0
96.00	7149.0
97.00	155.0
103.90	546.0
104.90	243.0
105.80	467.0
106.90	163.0
107.80	103.0
111.80	131.0
114.80	160.0
115.90	489.0
116.90	890.0
117.90	541.0
118.90	686.0
126.80	106.0
128.10	379.0
128.90	224.0
129.90	464.0
130.90	234.0
134.80	221.0
136.80	281.0
139.80	108.0
141.00	1328.0
142.00	224.0
142.90	1762.0
144.00	133.0
144.90	582.0
146.00	205.0
148.00	292.0
149.70	121.0
154.90	322.0
156.90	311.0
158.90	158.0
160.80	126.0
170.90	299.0
172.00	1360.0
173.00	1463.0
174.00	92088.0
175.00	6835.0
176.00	87712.0
177.00	5188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB307