

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025681.D
 Acq On : 22 Apr 2022 15:08
 Operator : SY/MD
 Sample : N2517-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH7

Quant Time: Apr 23 01:59:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.612	114	193886	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.850	117	193138	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.246	152	90627	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.310	65	104646	5.805	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	116.200%	
7) Chloroethane-d5		1.571	69	92165	4.806	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.200%	
11) 1,1-Dichloroethene-d2		2.108	63	154225	4.271	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.400%	
20) 2-Butanone-d5		3.889	46	119545	54.521	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.040%	
24) Chloroform-d		4.346	84	148132	5.438	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.800%	
26) 1,2-Dichloroethane-d4		5.027	65	68225	5.813	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	116.200%	
32) Benzene-d6		5.046	84	305145	5.461	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.200%	
36) 1,2-Dichloropropane-d6		6.066	67	88424	5.674	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.400%	
41) Toluene-d8		7.313	98	264351	5.098	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%	
43) trans-1,3-Dichloroprop...		7.622	79	26087	4.980	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.600%	
46) 2-Hexanone-d5		8.085	63	92090	50.090	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.180%	
56) 1,1,2,2-Tetrachloroeth...		10.213	84	46988	4.772	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4		11.622	152	81440	5.360	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%	
Target Compounds							
25) Chloroform		4.371	83	10749	0.427	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025681.D
Acq On : 22 Apr 2022 15:08
Operator : SY/MD
Sample : N2517-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH7

Quant Time: Apr 23 01:59:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

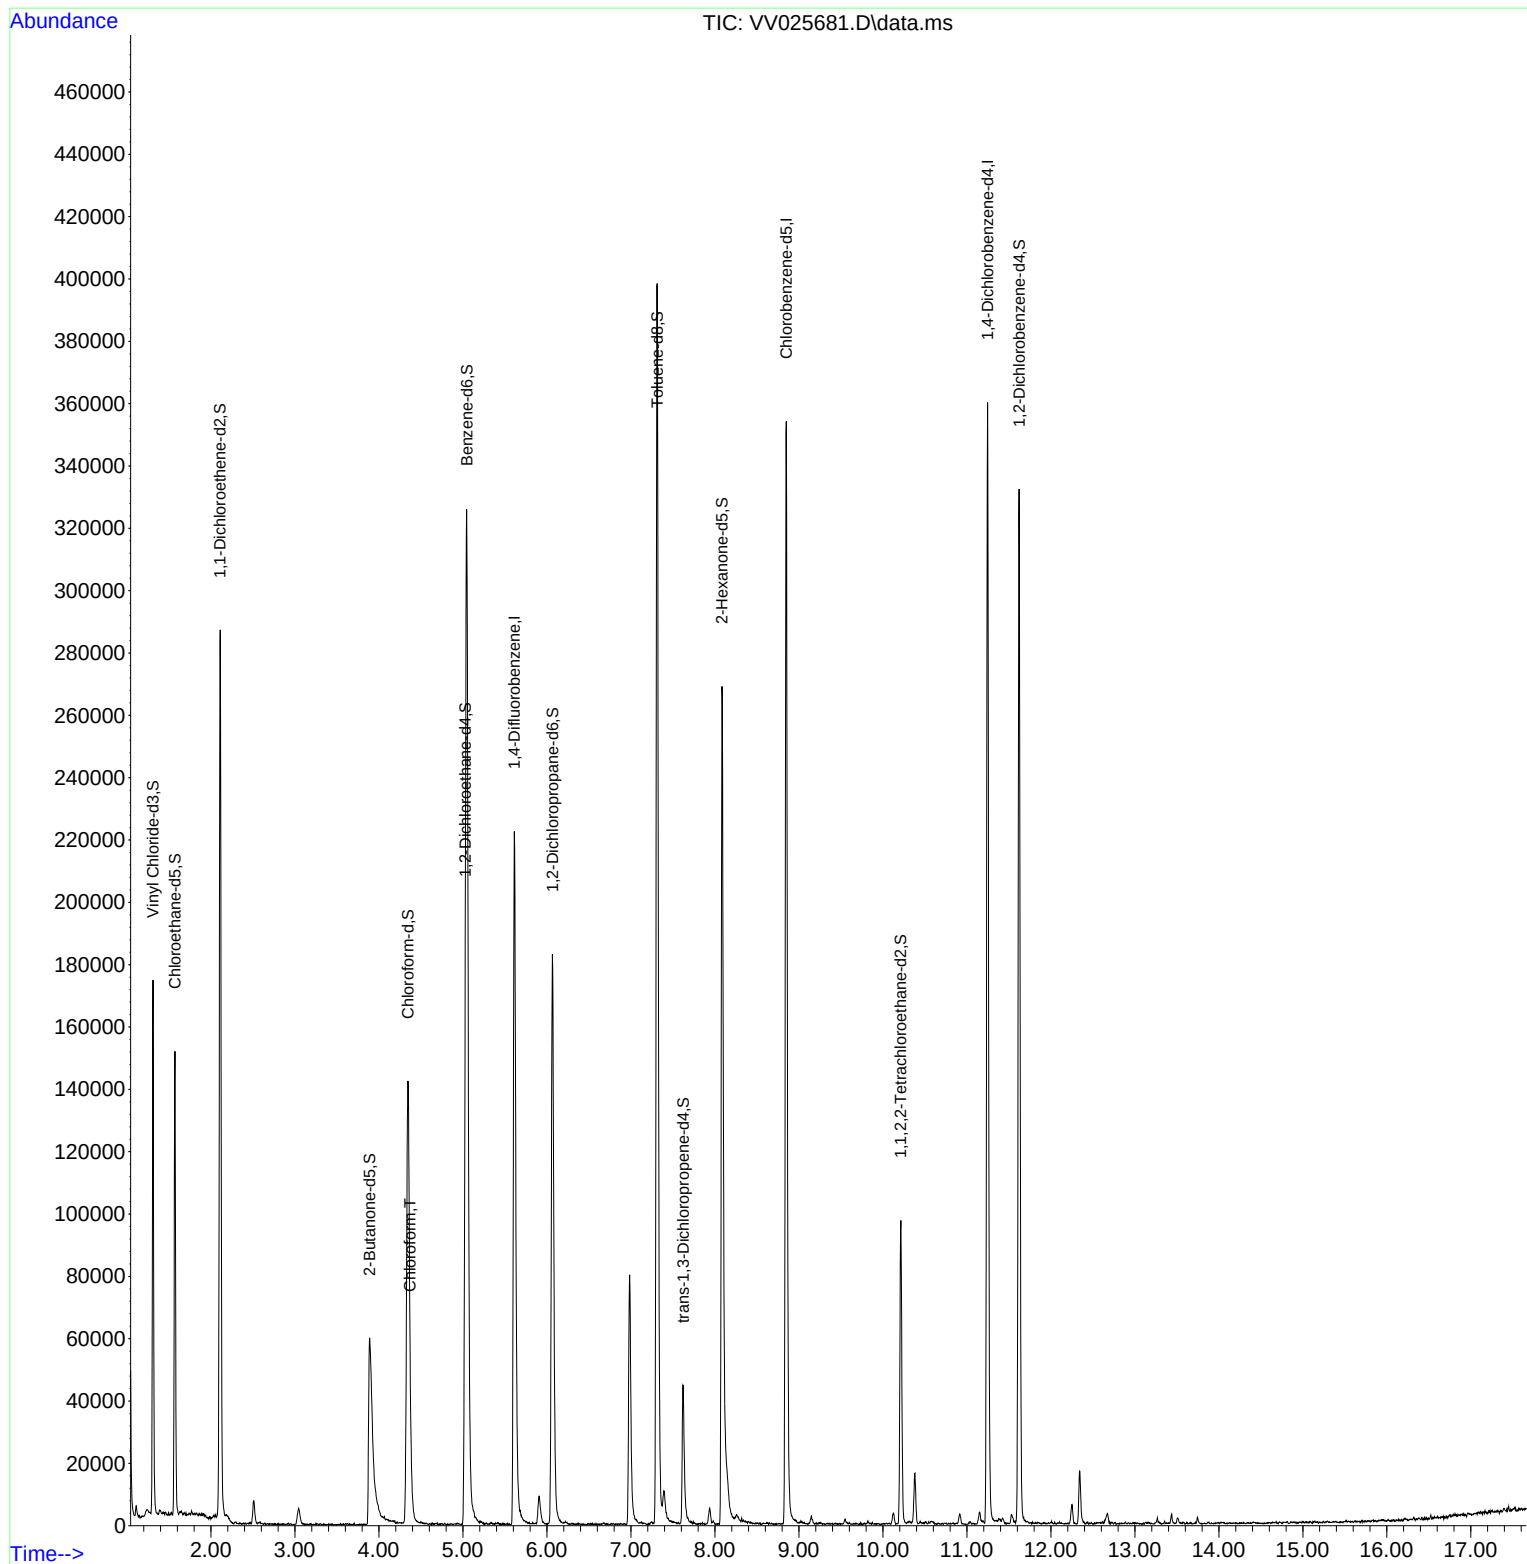

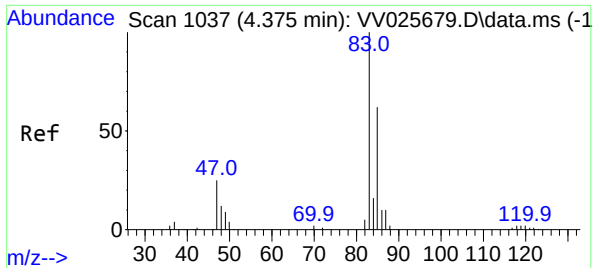

#25
 Chloroform
 Concen: 0.427 ug/L
 RT: 4.371 min Scan# 10
 Delta R.T. -0.000 min
 Lab File: VV025681.D
 Acq: 22 Apr 2022 15:08

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH7

Tgt Ion: 83 Resp: 10749

Ion	Ratio	Lower	Upper
83	100		
85	64.2	43.5	80.7

