

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025682.D
 Acq On : 22 Apr 2022 15:32
 Operator : SY/MD
 Sample : N2517-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH8

Quant Time: Apr 23 01:59:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	179286	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	182602	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	82899	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	94242	5.654	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.000%
7) Chloroethane-d5	1.571	69	81870	4.617	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.400%
11) 1,1-Dichloroethene-d2	2.111	63	140762	4.216	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.400%
20) 2-Butanone-d5	3.899	46	110089	54.297	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.600%
24) Chloroform-d	4.352	84	131812	5.233	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
26) 1,2-Dichloroethane-d4	5.034	65	59950	5.524	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.050	84	273232	5.172	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.400%
36) 1,2-Dichloropropane-d6	6.069	67	79023	5.363	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%
41) Toluene-d8	7.317	98	236624	4.826	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
43) trans-1,3-Dichloroprop...	7.625	79	23523	4.750	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.000%
46) 2-Hexanone-d5	8.088	63	81572	46.930	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.860%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43071	4.627	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	74860	5.386	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						
25) Chloroform	4.378	83	9192	0.395	ug/L	Qvalue # 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025682.D
Acq On : 22 Apr 2022 15:32
Operator : SY/MD
Sample : N2517-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFH8

Quant Time: Apr 23 01:59:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

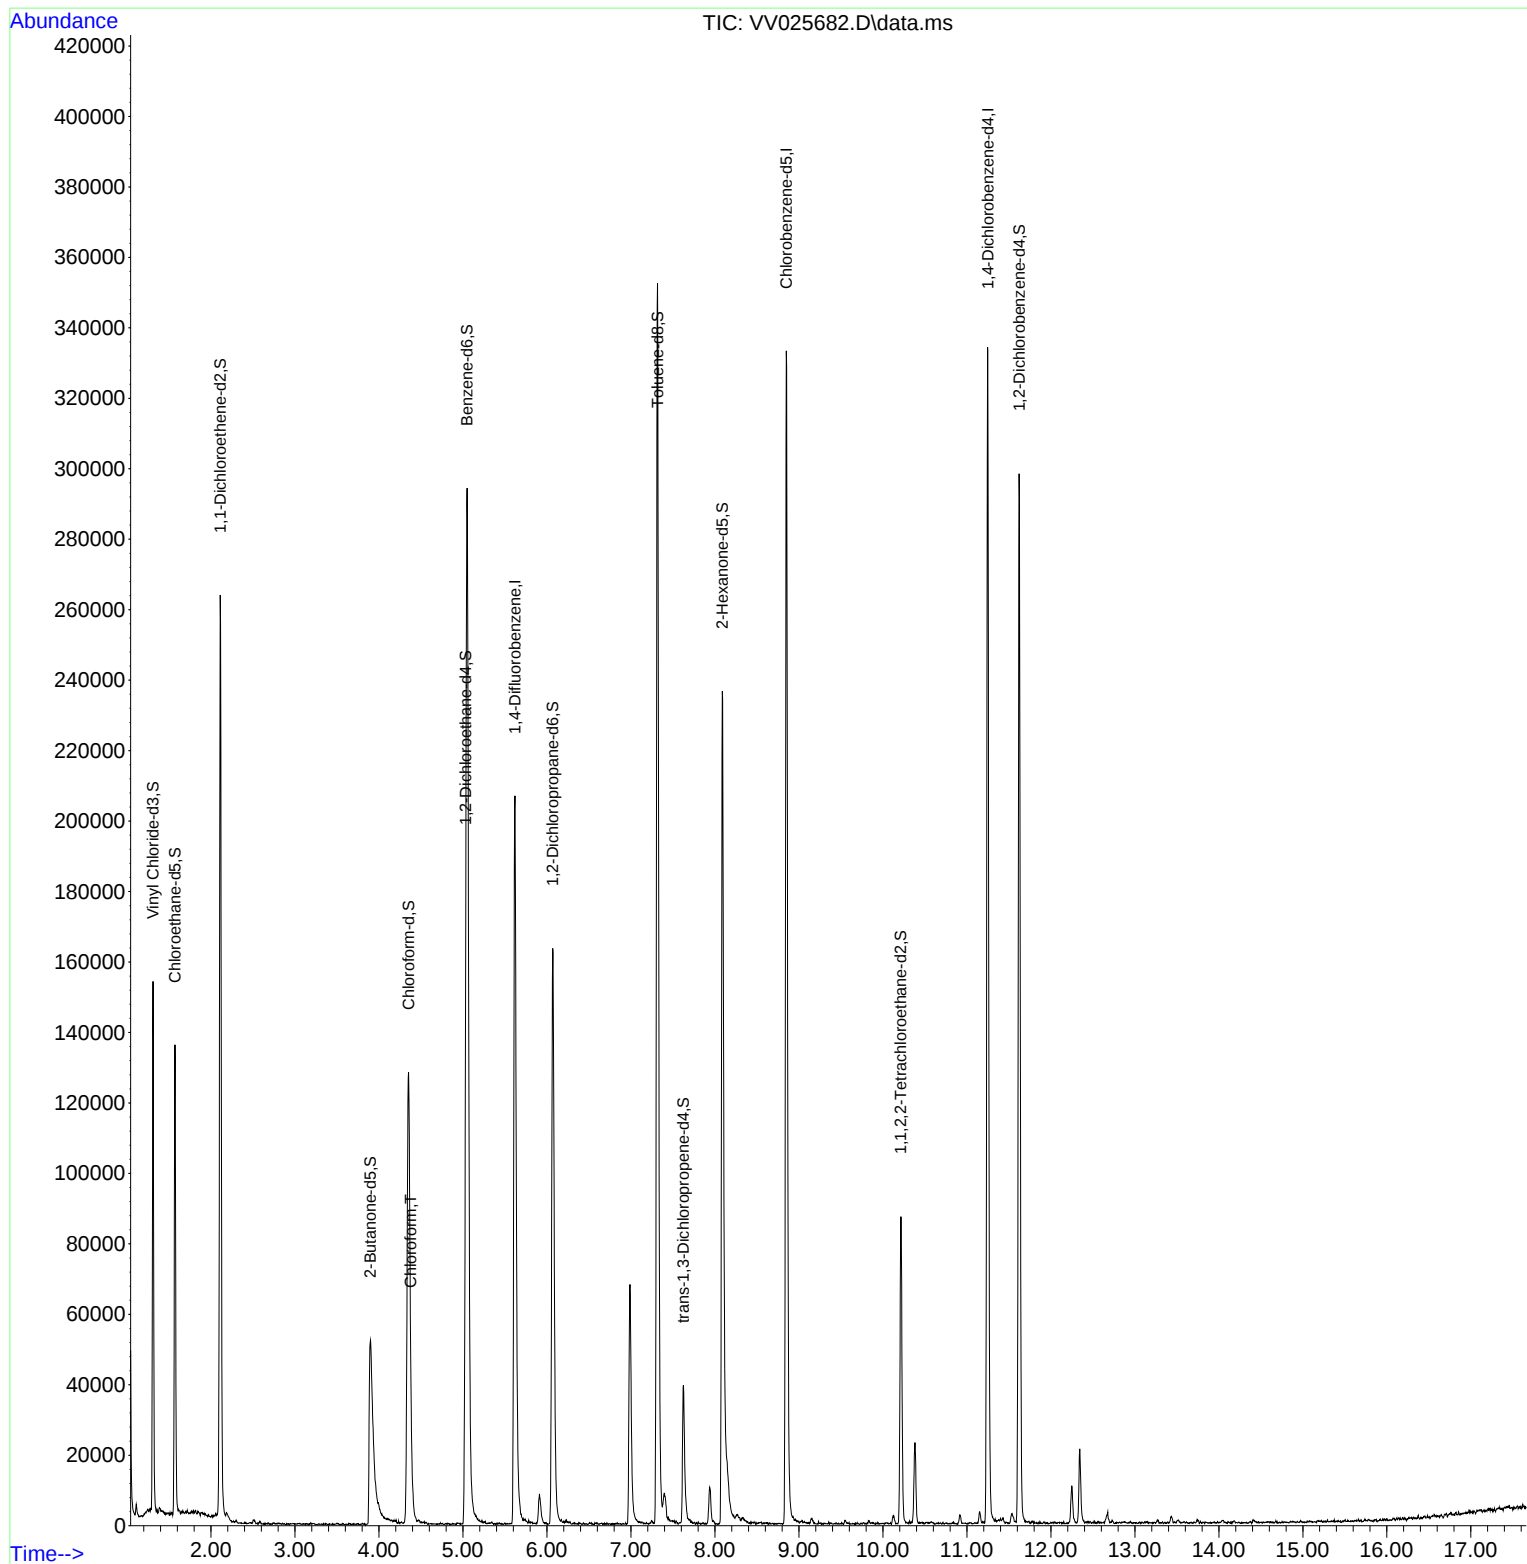

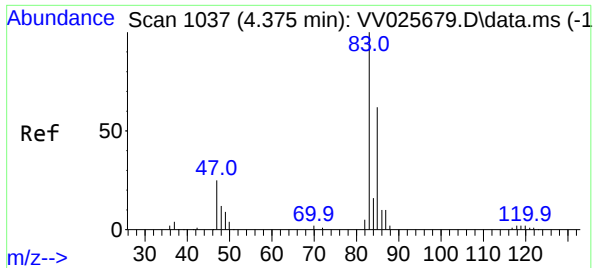

#25
 Chloroform
 Concen: 0.395 ug/L
 RT: 4.378 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV025682.D
 Acq: 22 Apr 2022 15:32

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFH8

Tgt Ion: 83 Resp: 9192
 Ion Ratio Lower Upper
 83 100
 85 85.1 43.5 80.7#

