

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025685.D
 Acq On : 22 Apr 2022 17:05
 Operator : SY/MD
 Sample : N2492-08DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W0DL

Quant Time: Apr 23 02:00:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129572	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	129626	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56207	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73517	6.103	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	122.000%	
7) Chloroethane-d5	1.571	69	68128	5.316	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.400%	
11) 1,1-Dichloroethene-d2	2.111	63	105803	4.384	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	87.600%	
20) 2-Butanone-d5	3.896	46	83197	56.777	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	113.560%	
24) Chloroform-d	4.352	84	106928	5.874	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	117.400%	
26) 1,2-Dichloroethane-d4	5.034	65	48042	6.125	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	122.600%	
32) Benzene-d6	5.053	84	217365	5.796	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.000%	
36) 1,2-Dichloropropane-d6	6.069	67	62990	6.022	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	120.400%	
41) Toluene-d8	7.317	98	179600	5.160	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.200%	
43) trans-1,3-Dichloroprop...	7.625	79	18011	5.123	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	102.400%	
46) 2-Hexanone-d5	8.088	63	63727	51.647	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.300%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35089	5.310	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	55524	5.892	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	117.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.513	84	2351	0.216	ug/L	91
47) Tetrachloroethene	7.976	164	28451	3.574	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025685.D
Acq On : 22 Apr 2022 17:05
Operator : SY/MD
Sample : N2492-08DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Quant Time: Apr 23 02:00:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration




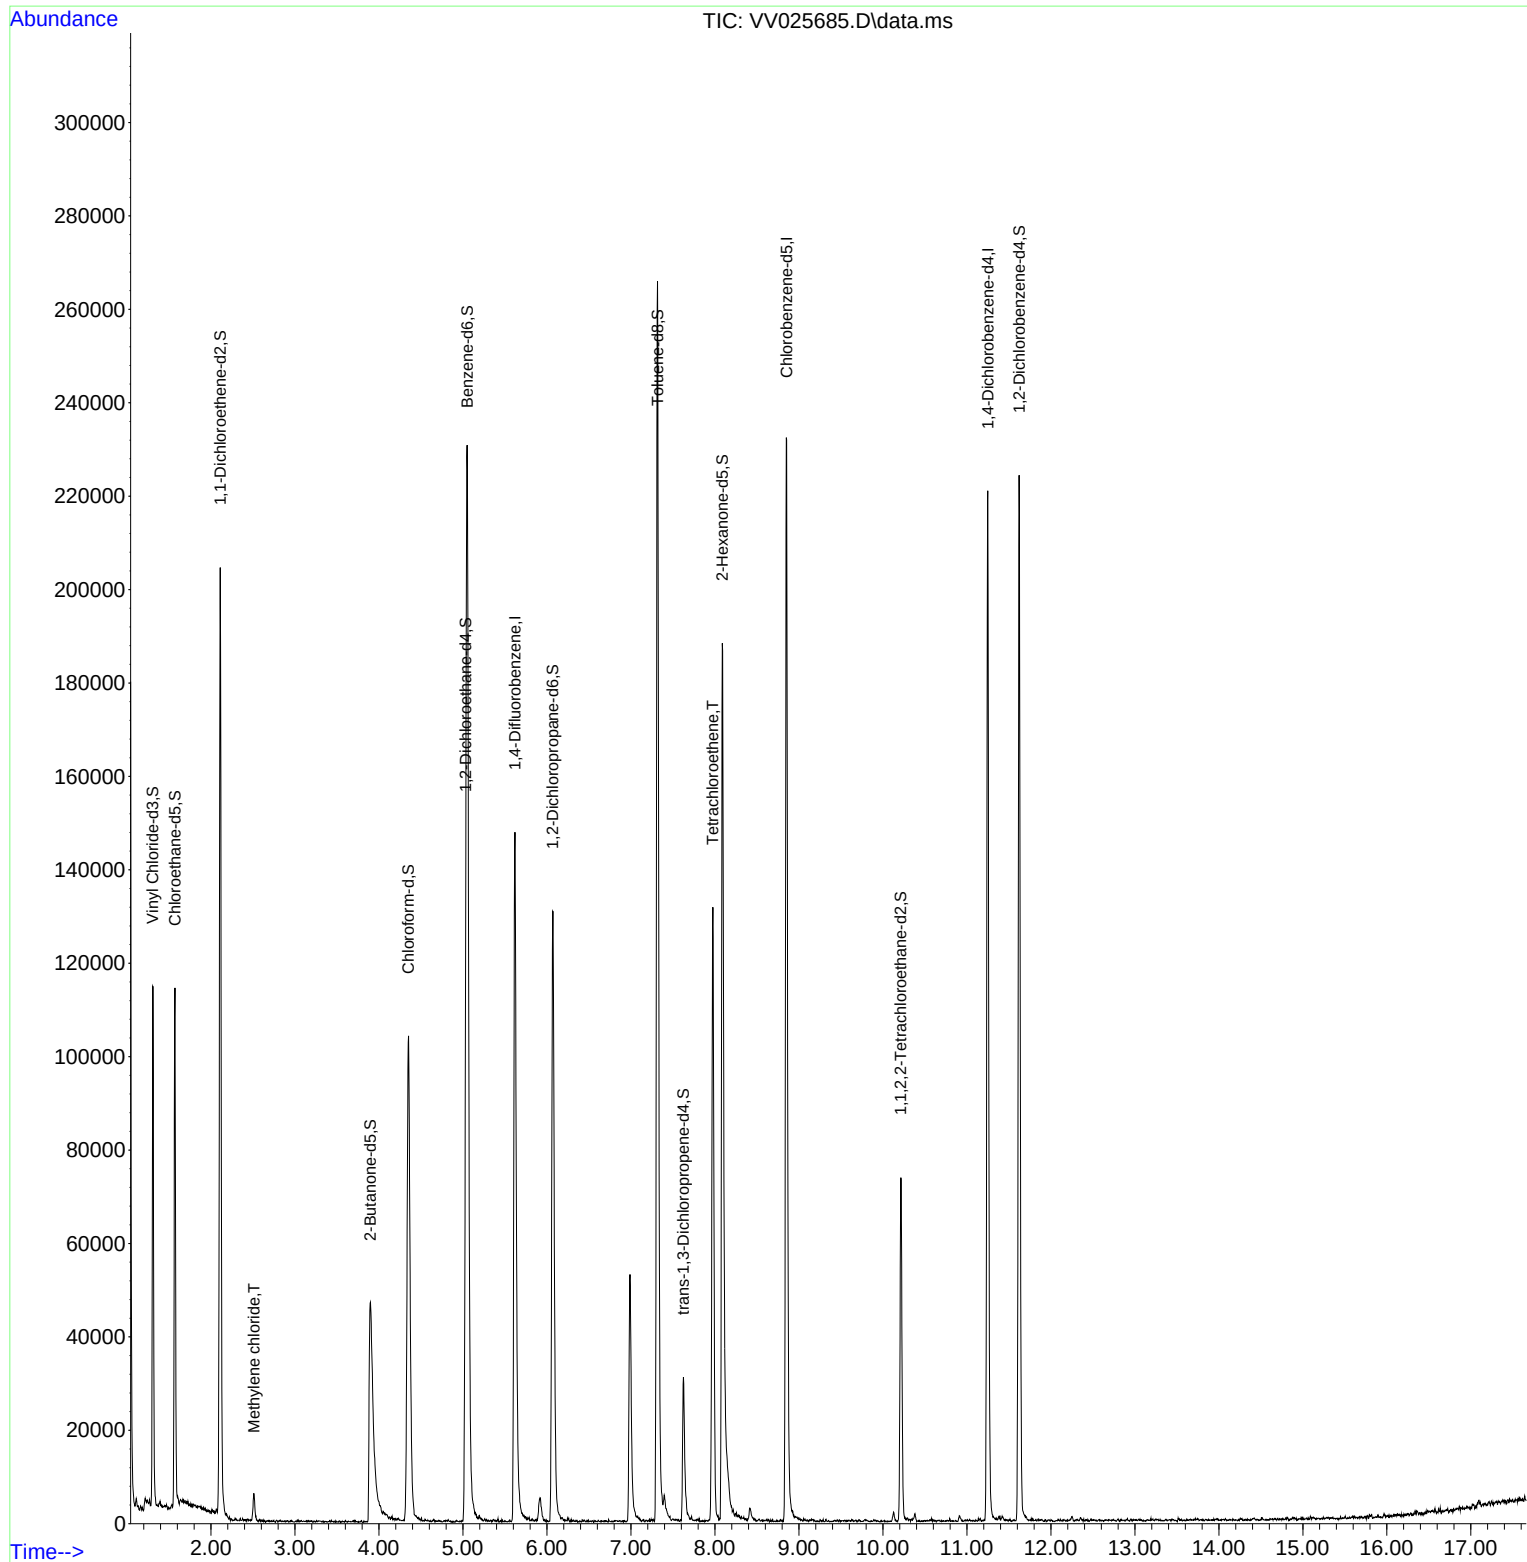


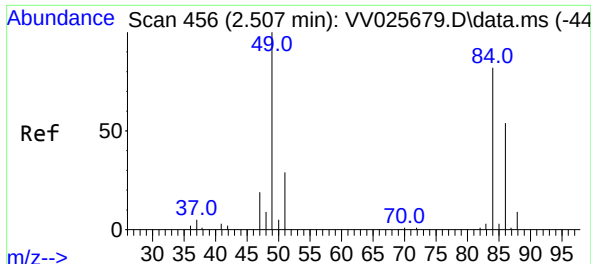

#16
Methylene chloride
Concen: 0.216 ug/L
RT: 2.513 min Scan# 41
Delta R.T. 0.007 min
Lab File: VV025685.D
Acq: 22 Apr 2022 17:05

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Tgt Ion: 84 Resp: 2351
Ion Ratio Lower Upper
84 100
86 62.6 45.9 85.3
49 122.0 76.6 142.3

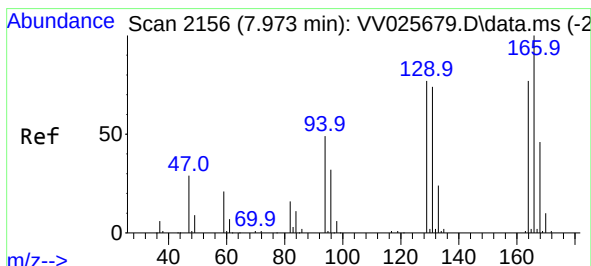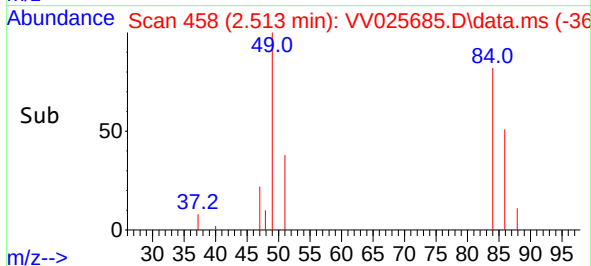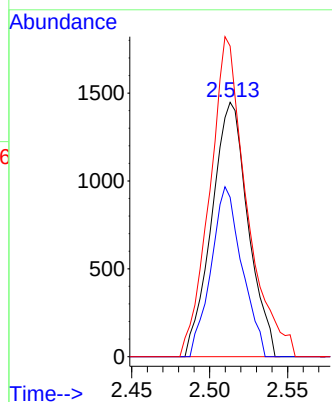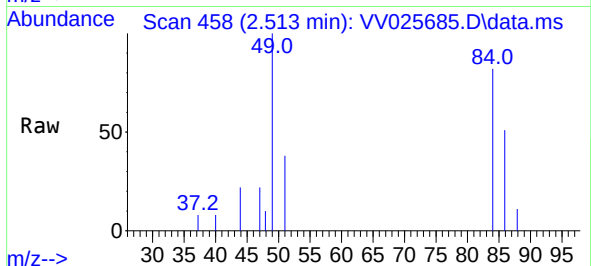

#47
Tetrachloroethene
Concen: 3.574 ug/L
RT: 7.976 min Scan# 2157
Delta R.T. 0.003 min
Lab File: VV025685.D
Acq: 22 Apr 2022 17:05

Tgt Ion:164 Resp: 28451
Ion Ratio Lower Upper
164 100
129 92.7 66.8 124.2
131 92.7 66.4 123.4
166 125.4 91.7 170.3

