

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025687.D
 Acq On : 22 Apr 2022 17:52
 Operator : SY/MD
 Sample : N2492-04DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T6DL

Quant Time: Apr 23 02:01:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	126530	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56159	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	77784	6.612	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 132.200%#		
7) Chloroethane-d5	1.571	69	69082	5.520	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 110.400%		
11) 1,1-Dichloroethene-d2	2.111	63	114707	4.868	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 97.400%		
20) 2-Butanone-d5	3.902	46	91994	64.290	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	= 128.580%		
24) Chloroform-d	4.352	84	111127	6.251	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 125.000%		
26) 1,2-Dichloroethane-d4	5.034	65	50765	6.628	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 132.600%#		
32) Benzene-d6	5.053	84	222545	6.117	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 122.400%		
36) 1,2-Dichloropropane-d6	6.072	67	66210	6.526	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 130.600%		
41) Toluene-d8	7.317	98	190844	5.653	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 113.000%		
43) trans-1,3-Dichloroprop...	7.625	79	18684	5.479	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 109.600%		
46) 2-Hexanone-d5	8.091	63	63428	52.993	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 105.980%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37177	5.800	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 116.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	59136	6.281	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 125.600%#		
Target Compounds						Qvalue
47) Tetrachloroethene	7.979	164	14838	1.922	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025687.D
Acq On : 22 Apr 2022 17:52
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Time: Apr 23 02:01:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

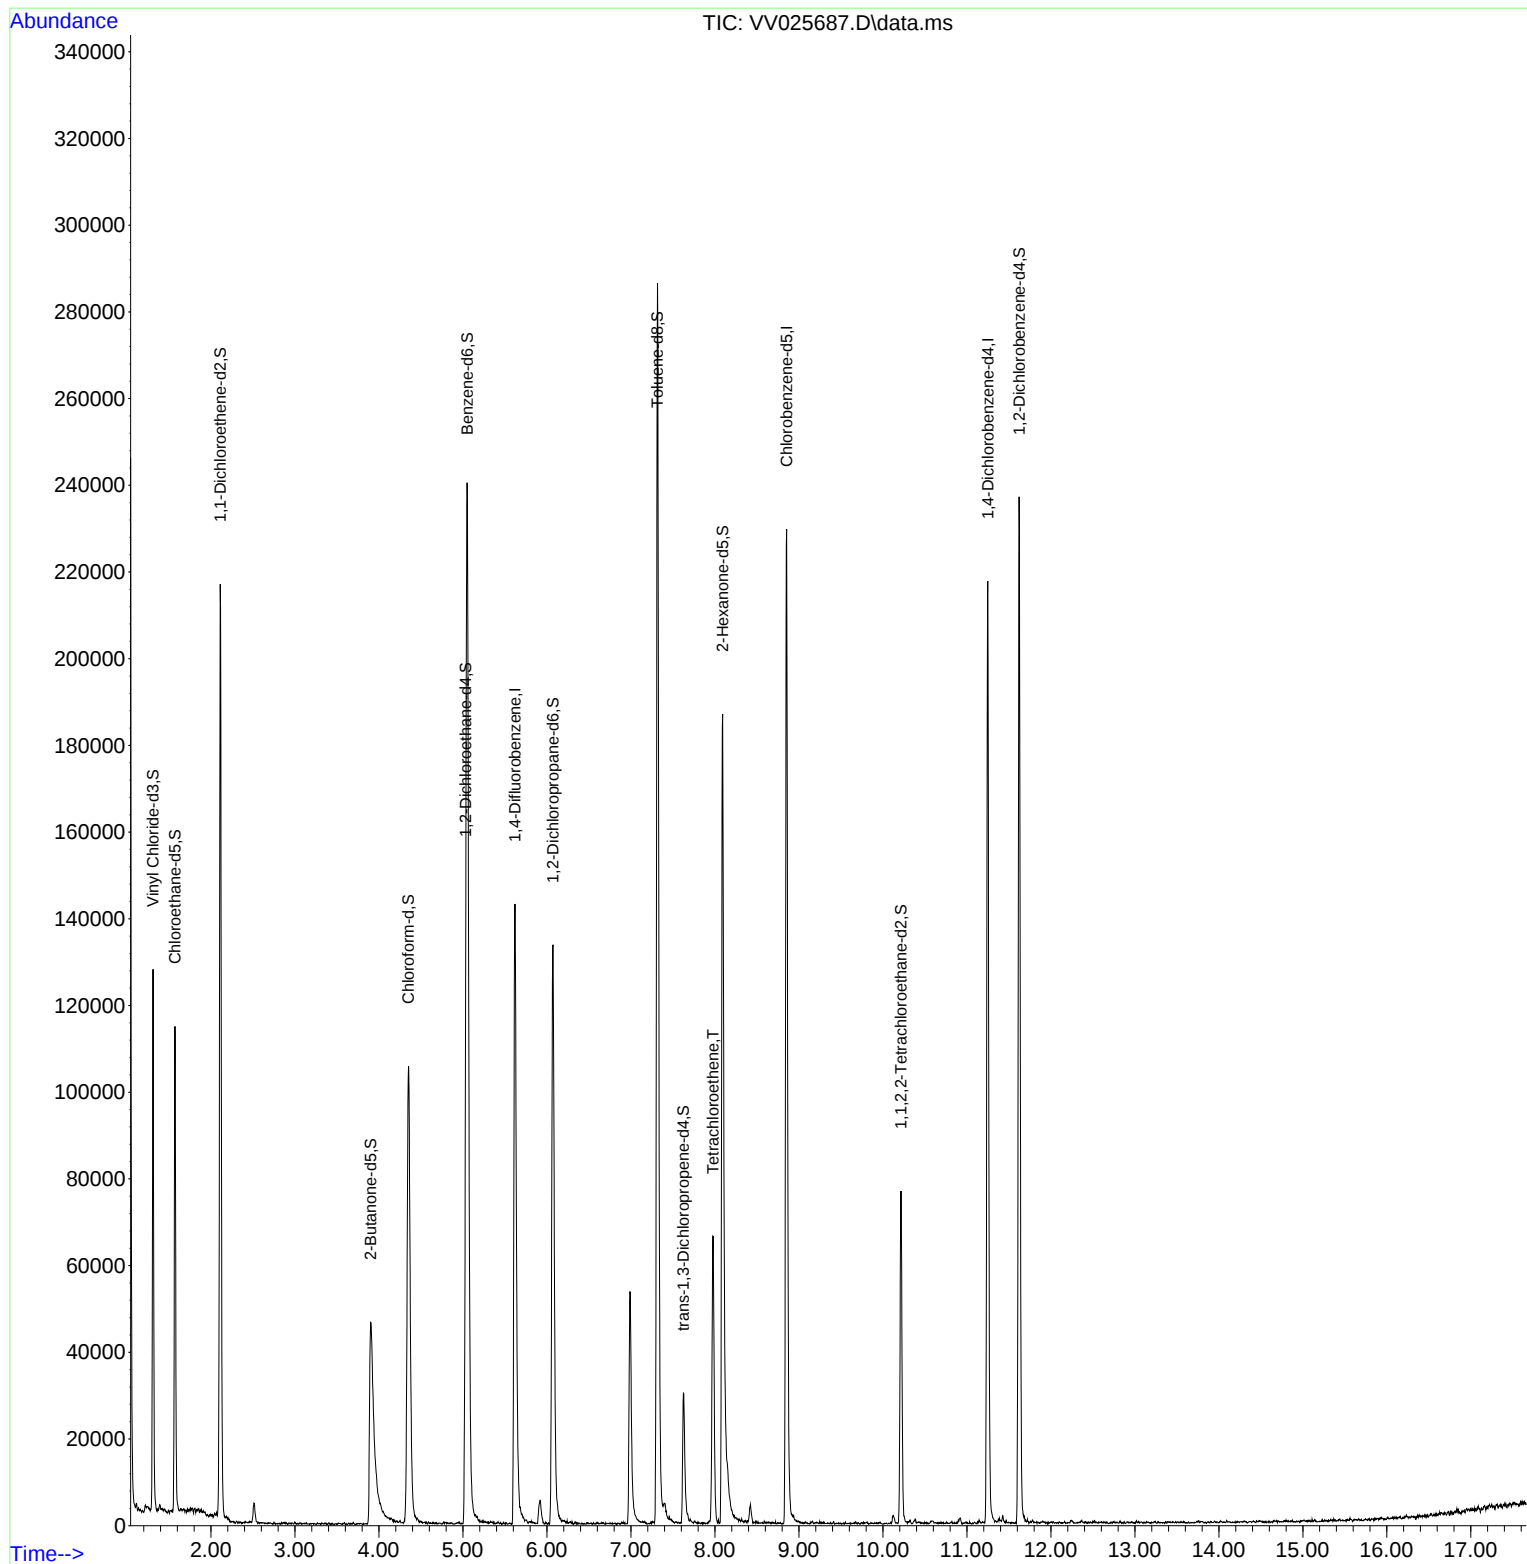

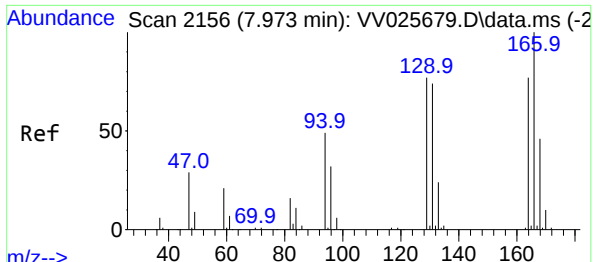

#47
Tetrachloroethene
Concen: 1.922 ug/L
RT: 7.979 min Scan# 2156
Delta R.T. 0.006 min
Lab File: VV025687.D
Acq: 22 Apr 2022 17:52

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Tgt Ion:164 Resp: 14838

Ion	Ratio	Lower	Upper
164	100		
129	98.2	66.8	124.2
131	94.4	66.4	123.4
166	127.2	91.7	170.3

