

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025693.D
 Acq On : 22 Apr 2022 20:13
 Operator : SY/MD
 Sample : N2492-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W7

Quant Time: Apr 23 02:02:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123358	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	128215	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	55361	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	69446	6.055	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 121.200%		
7) Chloroethane-d5	1.574	69	63033	5.166	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 103.400%		
11) 1,1-Dichloroethene-d2	2.111	63	102711	4.471	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 89.400%		
20) 2-Butanone-d5	3.899	46	85363	61.190	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 122.380%		
24) Chloroform-d	4.352	84	103445	5.969	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 119.400%		
26) 1,2-Dichloroethane-d4	5.037	65	47228	6.325	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 126.400%		
32) Benzene-d6	5.053	84	206490	5.566	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 111.400%		
36) 1,2-Dichloropropane-d6	6.072	67	61711	5.965	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 119.200%		
41) Toluene-d8	7.317	98	172457	5.009	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 100.200%		
43) trans-1,3-Dichloroprop...	7.625	79	17486	5.028	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 100.600%		
46) 2-Hexanone-d5	8.088	63	62426	51.149	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 102.300%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	34166	5.227	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 104.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	53241	5.736	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 114.800%		
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	113328	14.395	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025693.D
Acq On : 22 Apr 2022 20:13
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7


Quant Time: Apr 23 02:02:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

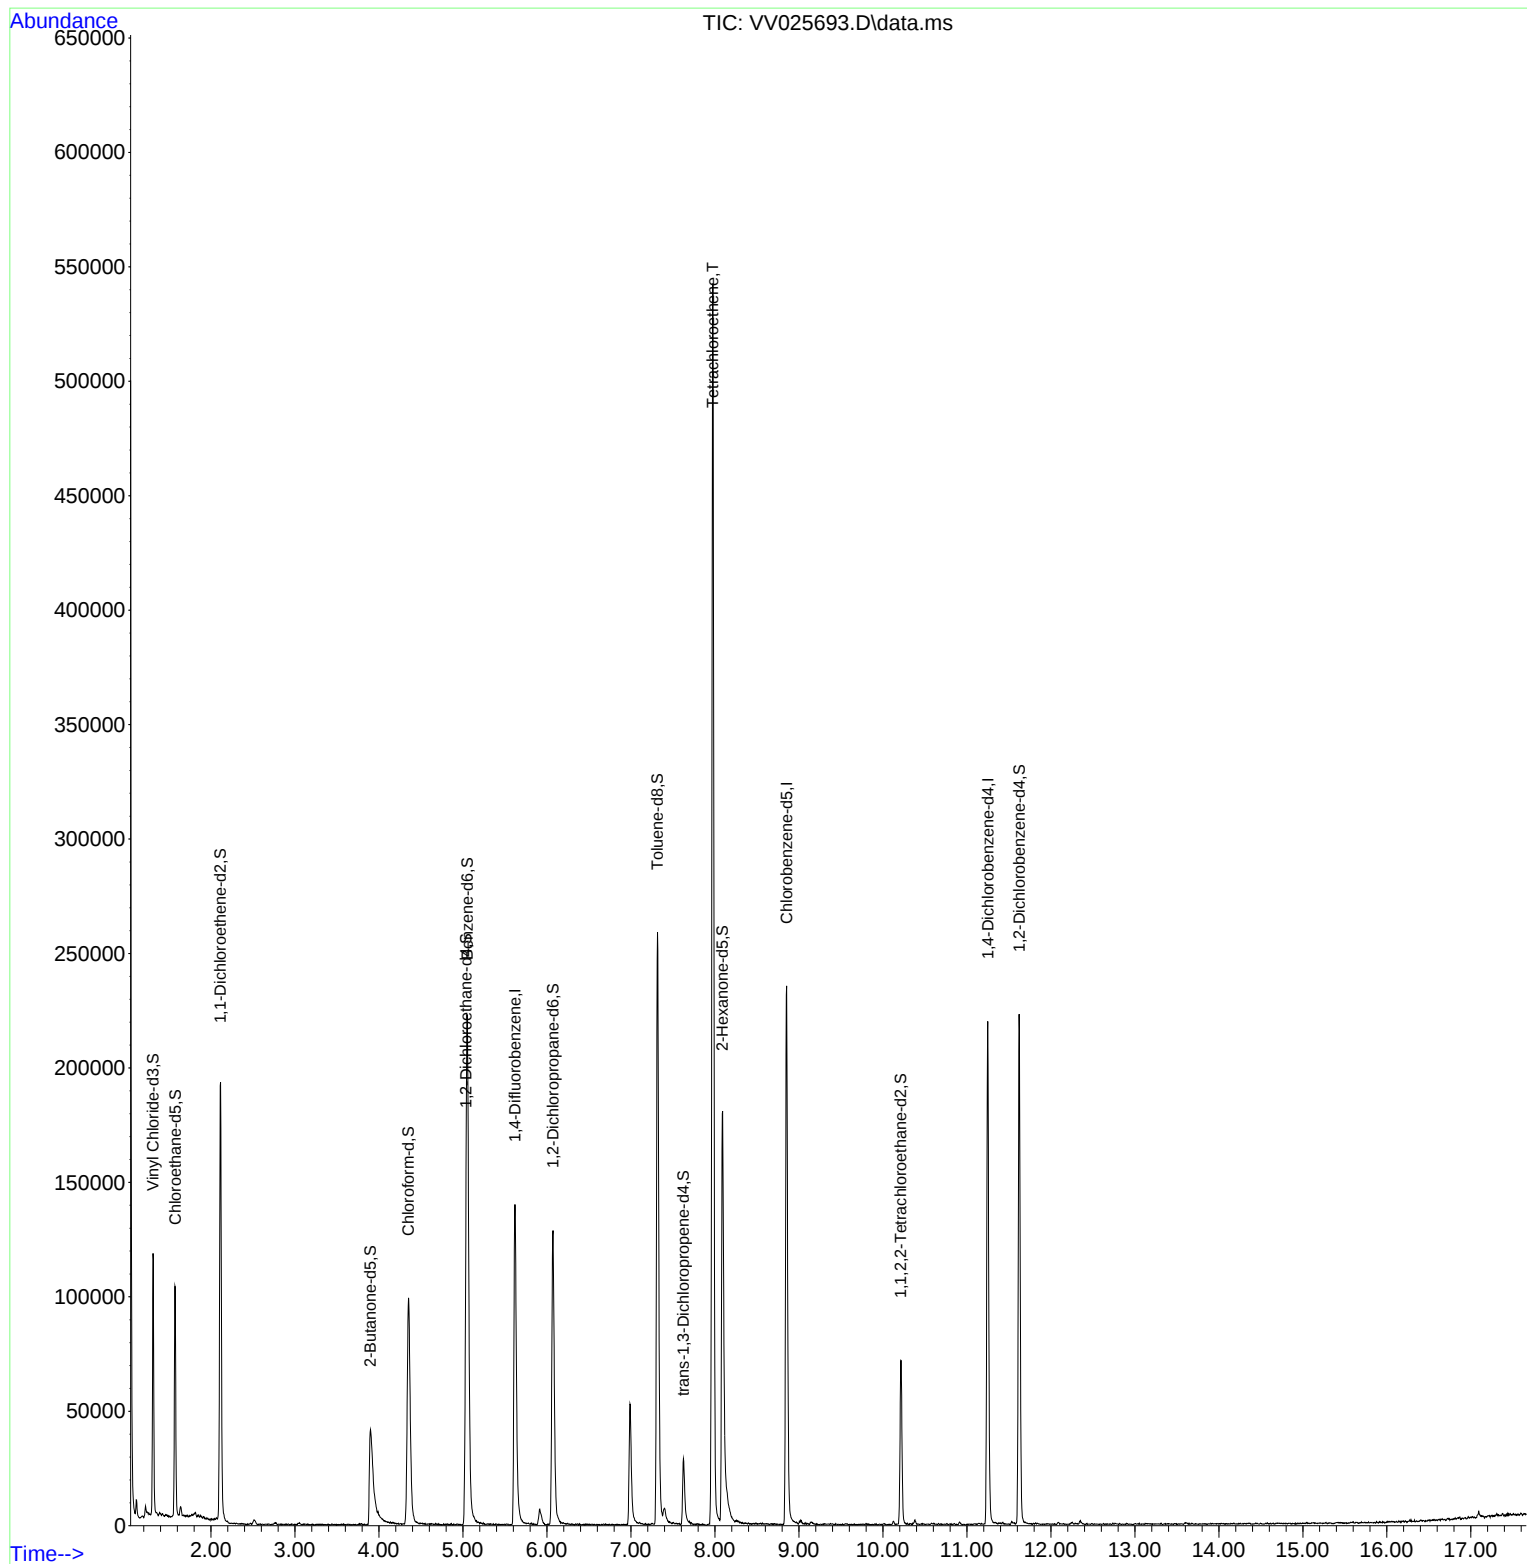

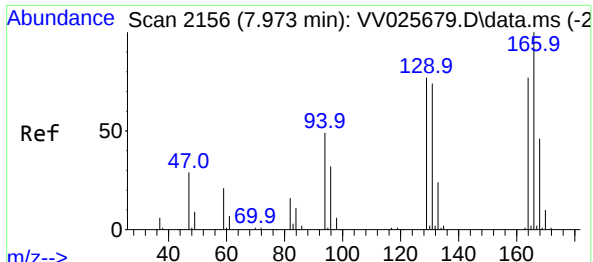

#47
 Tetrachloroethene
 Concen: 14.395 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV025693.D
 Acq: 22 Apr 2022 20:13

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W7

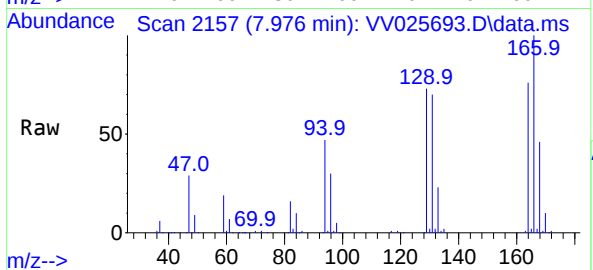

Tgt Ion:164 Resp: 113328

Ion	Ratio	Lower	Upper
164	100		
129	96.0	66.8	124.2
131	92.6	66.4	123.4
166	131.4	91.7	170.3

