

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025694.D
 Acq On : 22 Apr 2022 20:36
 Operator : SY/MD
 Sample : N2492-22
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W8

Quant Time: Apr 23 02:02:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117643	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124104	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	54132	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	69301	6.336	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.800%
7) Chloroethane-d5	1.574	69	63445	5.453	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.000%
11) 1,1-Dichloroethene-d2	2.114	63	104508	4.770	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.400%
20) 2-Butanone-d5	3.902	46	85190	64.032	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.060%
24) Chloroform-d	4.355	84	102861	6.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	124.400%
26) 1,2-Dichloroethane-d4	5.037	65	47729	6.702	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	134.000%#
32) Benzene-d6	5.053	84	209201	5.826	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.600%
36) 1,2-Dichloropropane-d6	6.072	67	60448	6.036	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	120.800%
41) Toluene-d8	7.317	98	171011	5.132	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
43) trans-1,3-Dichloroprop...	7.625	79	17815	5.293	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	105.800%
46) 2-Hexanone-d5	8.088	63	64499	54.598	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.200%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35625	5.631	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	53268	5.869	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.400%
Target Compounds						
					Qvalue	
47) Tetrachloroethene	7.976	164	338508	44.421	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025694.D
Acq On : 22 Apr 2022 20:36
Operator : SY/MD
Sample : N2492-22
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W8

Quant Time: Apr 23 02:02:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

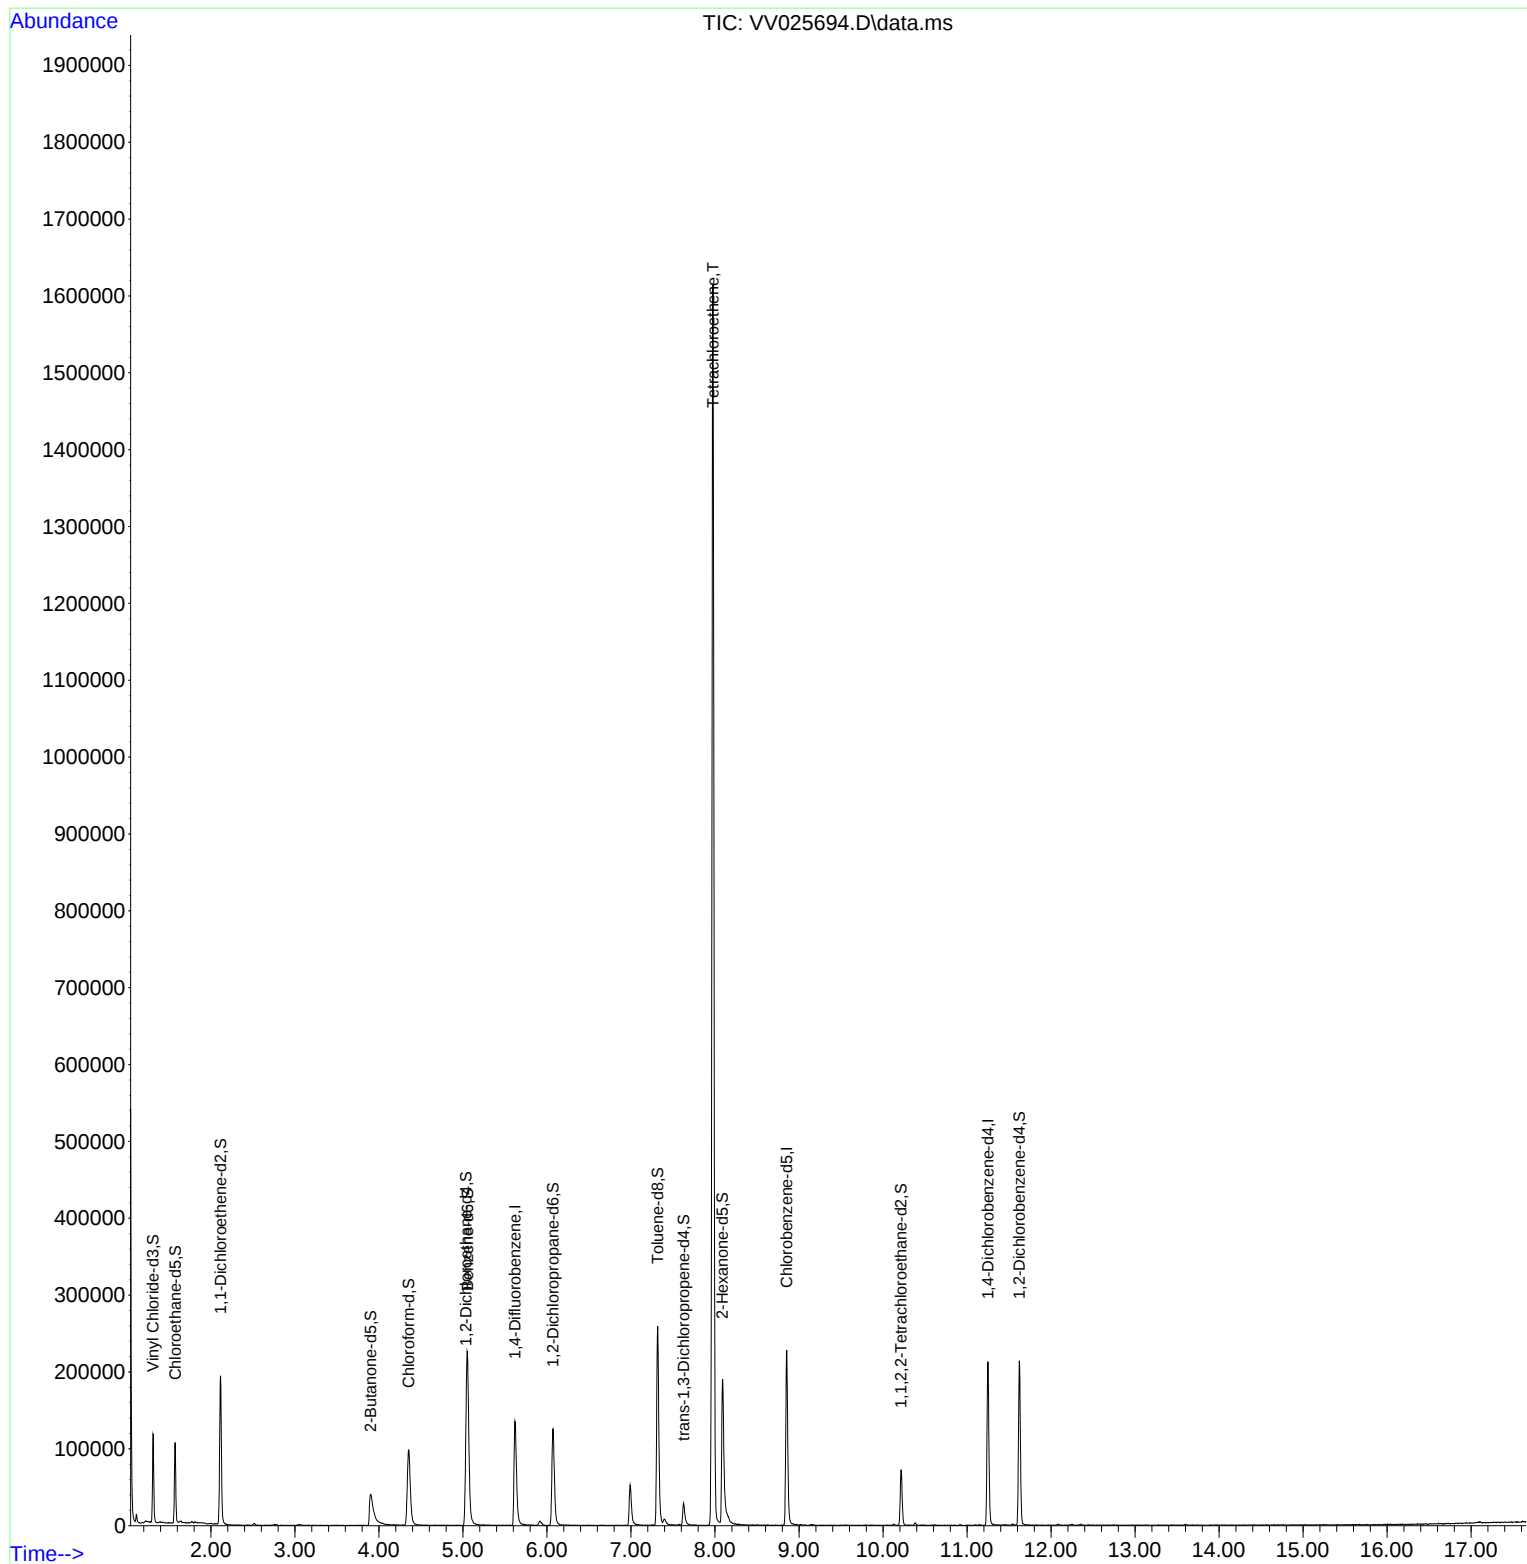

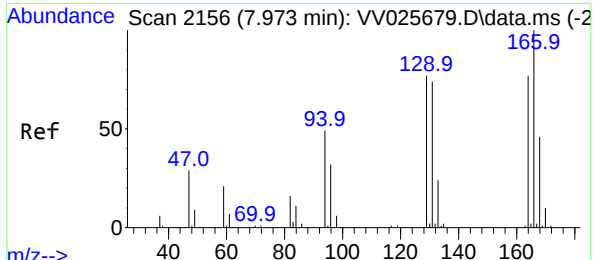

#47
 Tetrachloroethene
 Concen: 44.421 ug/L
 RT: 7.976 min Scan# 2156
 Delta R.T. 0.003 min
 Lab File: VV025694.D
 Acq: 22 Apr 2022 20:36

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W8

Tgt Ion:164 Resp: 338508

Ion	Ratio	Lower	Upper
164	100		
129	96.4	66.8	124.2
131	93.0	66.4	123.4
166	124.7	91.7	170.3

