

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025695.D
 Acq On : 22 Apr 2022 20:59
 Operator : SY/MD
 Sample : N2492-23
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W9

Quant Time: Apr 23 02:03:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	115786	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	122151	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	51542	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	72518	6.737	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	134.800%#
7) Chloroethane-d5	1.571	69	66195	5.780	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.600%
11) 1,1-Dichloroethene-d2	2.111	63	104046	4.825	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	96.400%
20) 2-Butanone-d5	3.899	46	85155	65.032	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	130.060%#
24) Chloroform-d	4.352	84	103390	6.356	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	127.200%#
26) 1,2-Dichloroethane-d4	5.037	65	48637	6.939	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	138.800%#
32) Benzene-d6	5.053	84	208180	5.890	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.800%
36) 1,2-Dichloropropane-d6	6.072	67	62593	6.350	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	127.000%
41) Toluene-d8	7.317	98	168762	5.145	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
43) trans-1,3-Dichloroprop...	7.625	79	17893	5.401	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	108.000%
46) 2-Hexanone-d5	8.088	63	64086	55.116	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.240%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35034	5.626	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	52828	6.113	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.200%#
Target Compounds						Qvalue
47) Tetrachloroethene	7.976	164	350494	46.729	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025695.D
Acq On : 22 Apr 2022 20:59
Operator : SY/MD
Sample : N2492-23
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W9

Quant Time: Apr 23 02:03:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

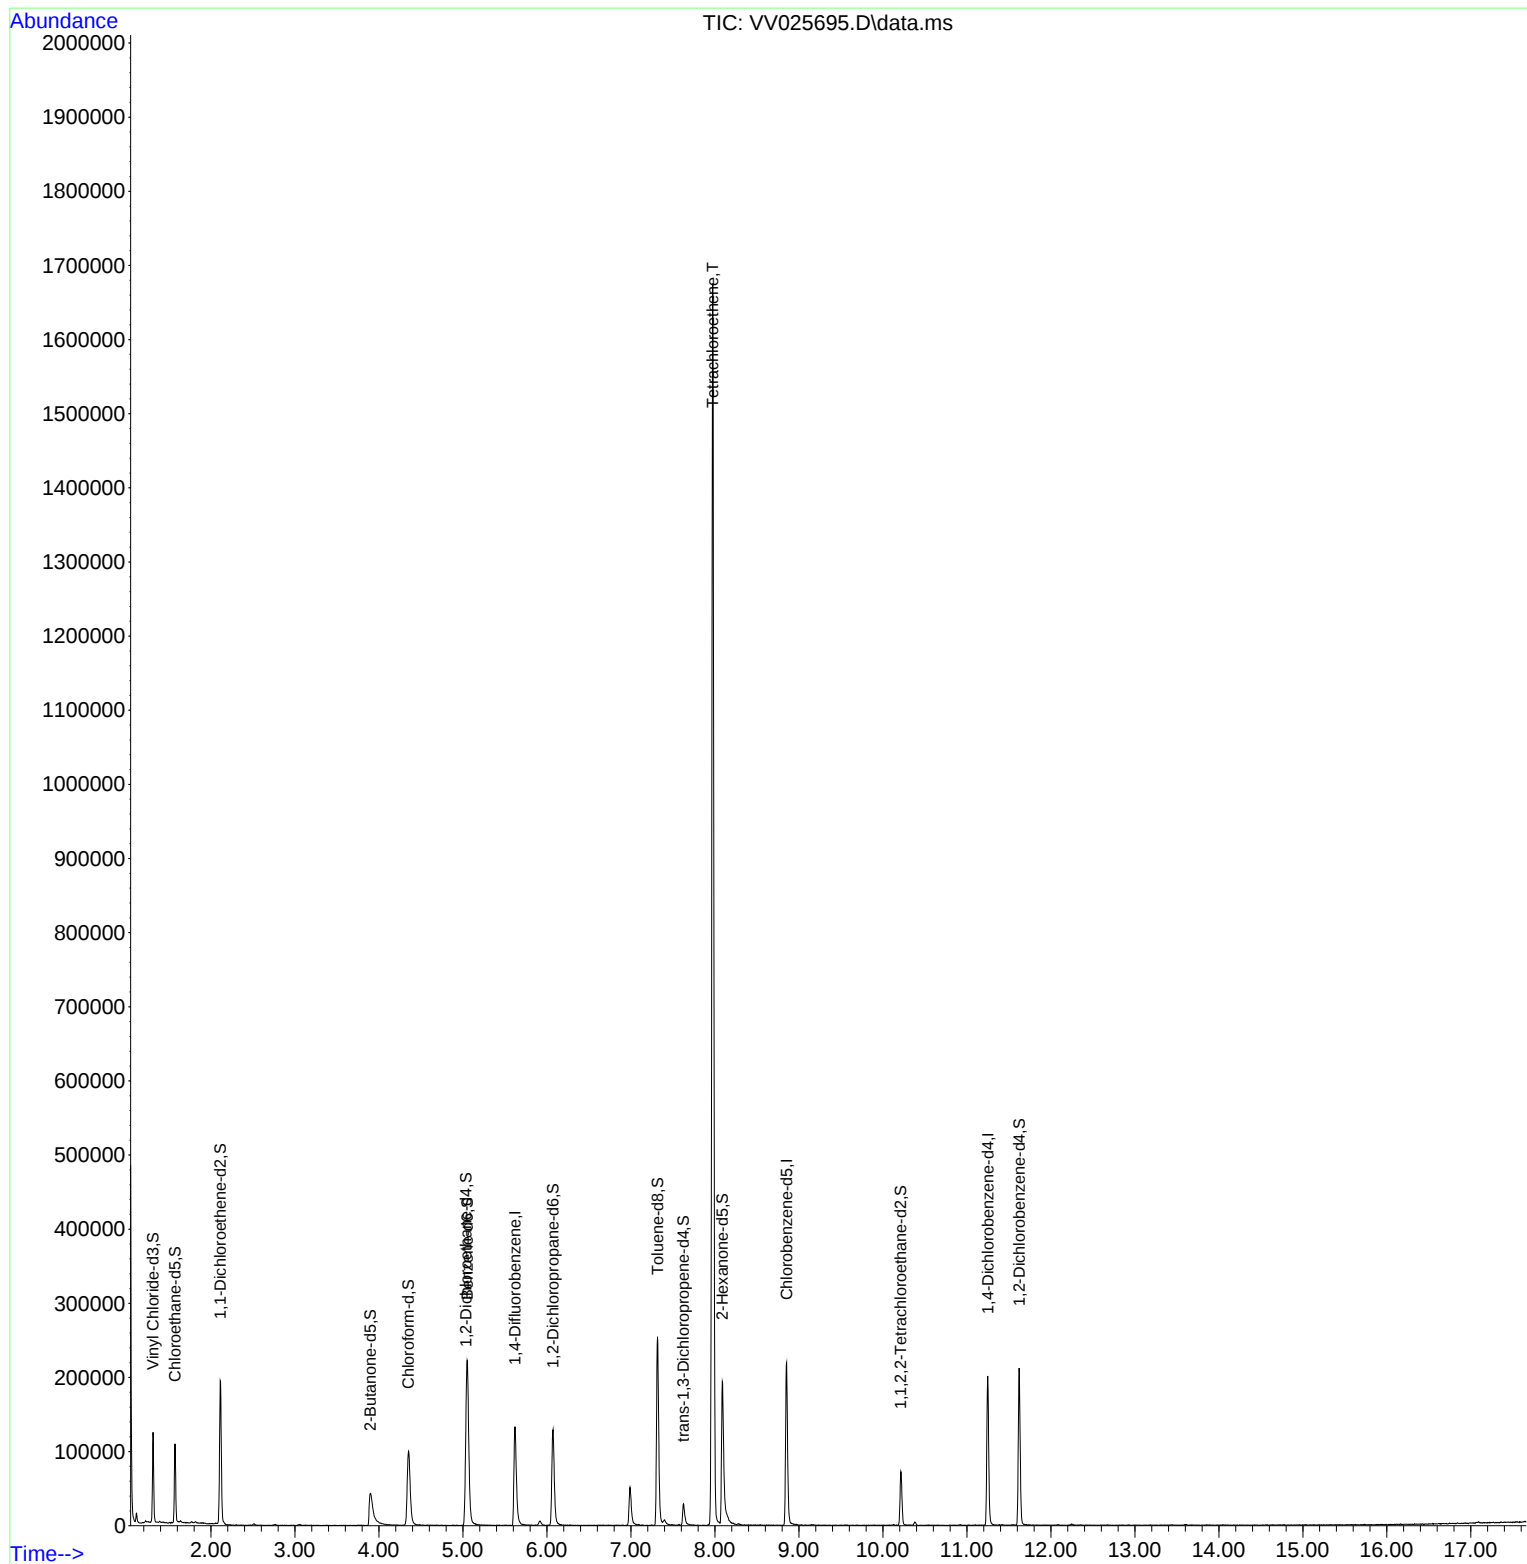

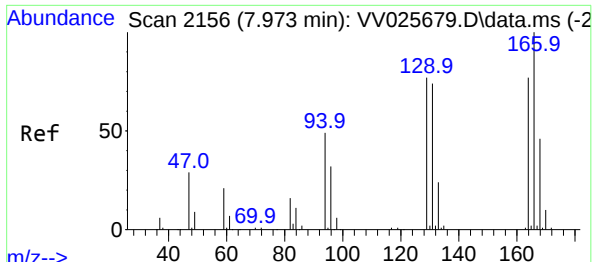

#47
 Tetrachloroethene
 Concen: 46.729 ug/L
 RT: 7.976 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VV025695.D
 Acq: 22 Apr 2022 20:59

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W9

Tgt Ion:164 Resp: 350494

Ion	Ratio	Lower	Upper
164	100		
129	98.4	66.8	124.2
131	92.8	66.4	123.4
166	127.5	91.7	170.3

