

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042222\
 Data File : VW025698.D
 Acq On : 22 Apr 2022 22:10
 Operator : SY/MD
 Sample : N2530-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X2

Quant Time: Apr 23 02:03:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 23 01:57:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	173008	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	174425	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	74516	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	94559	5.879	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	117.600%
7) Chloroethane-d5	1.574	69	87537	5.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.400%
11) 1,1-Dichloroethene-d2	2.114	63	140741	4.368	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.400%
20) 2-Butanone-d5	3.896	46	120240	61.455	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.920%
24) Chloroform-d	4.352	84	143449	5.902	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.000%
26) 1,2-Dichloroethane-d4	5.034	65	66151	6.316	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.400%
32) Benzene-d6	5.053	84	291215	5.770	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	115.400%
36) 1,2-Dichloropropane-d6	6.072	67	86330	6.134	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	122.600%
41) Toluene-d8	7.317	98	245621	5.244	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
43) trans-1,3-Dichloroprop...	7.625	79	25469	5.384	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.600%
46) 2-Hexanone-d5	8.088	63	90372	54.430	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.860%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48416	5.445	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	74786	5.986	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	119.800%
Target Compounds						Qvalue
47) Tetrachloroethene	7.979	164	4433	0.414	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025698.D
Acq On : 22 Apr 2022 22:10
Operator : SY/MD
Sample : N2530-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6X2

Quant Time: Apr 23 02:03:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 23 01:57:52 2022
Response via : Initial Calibration

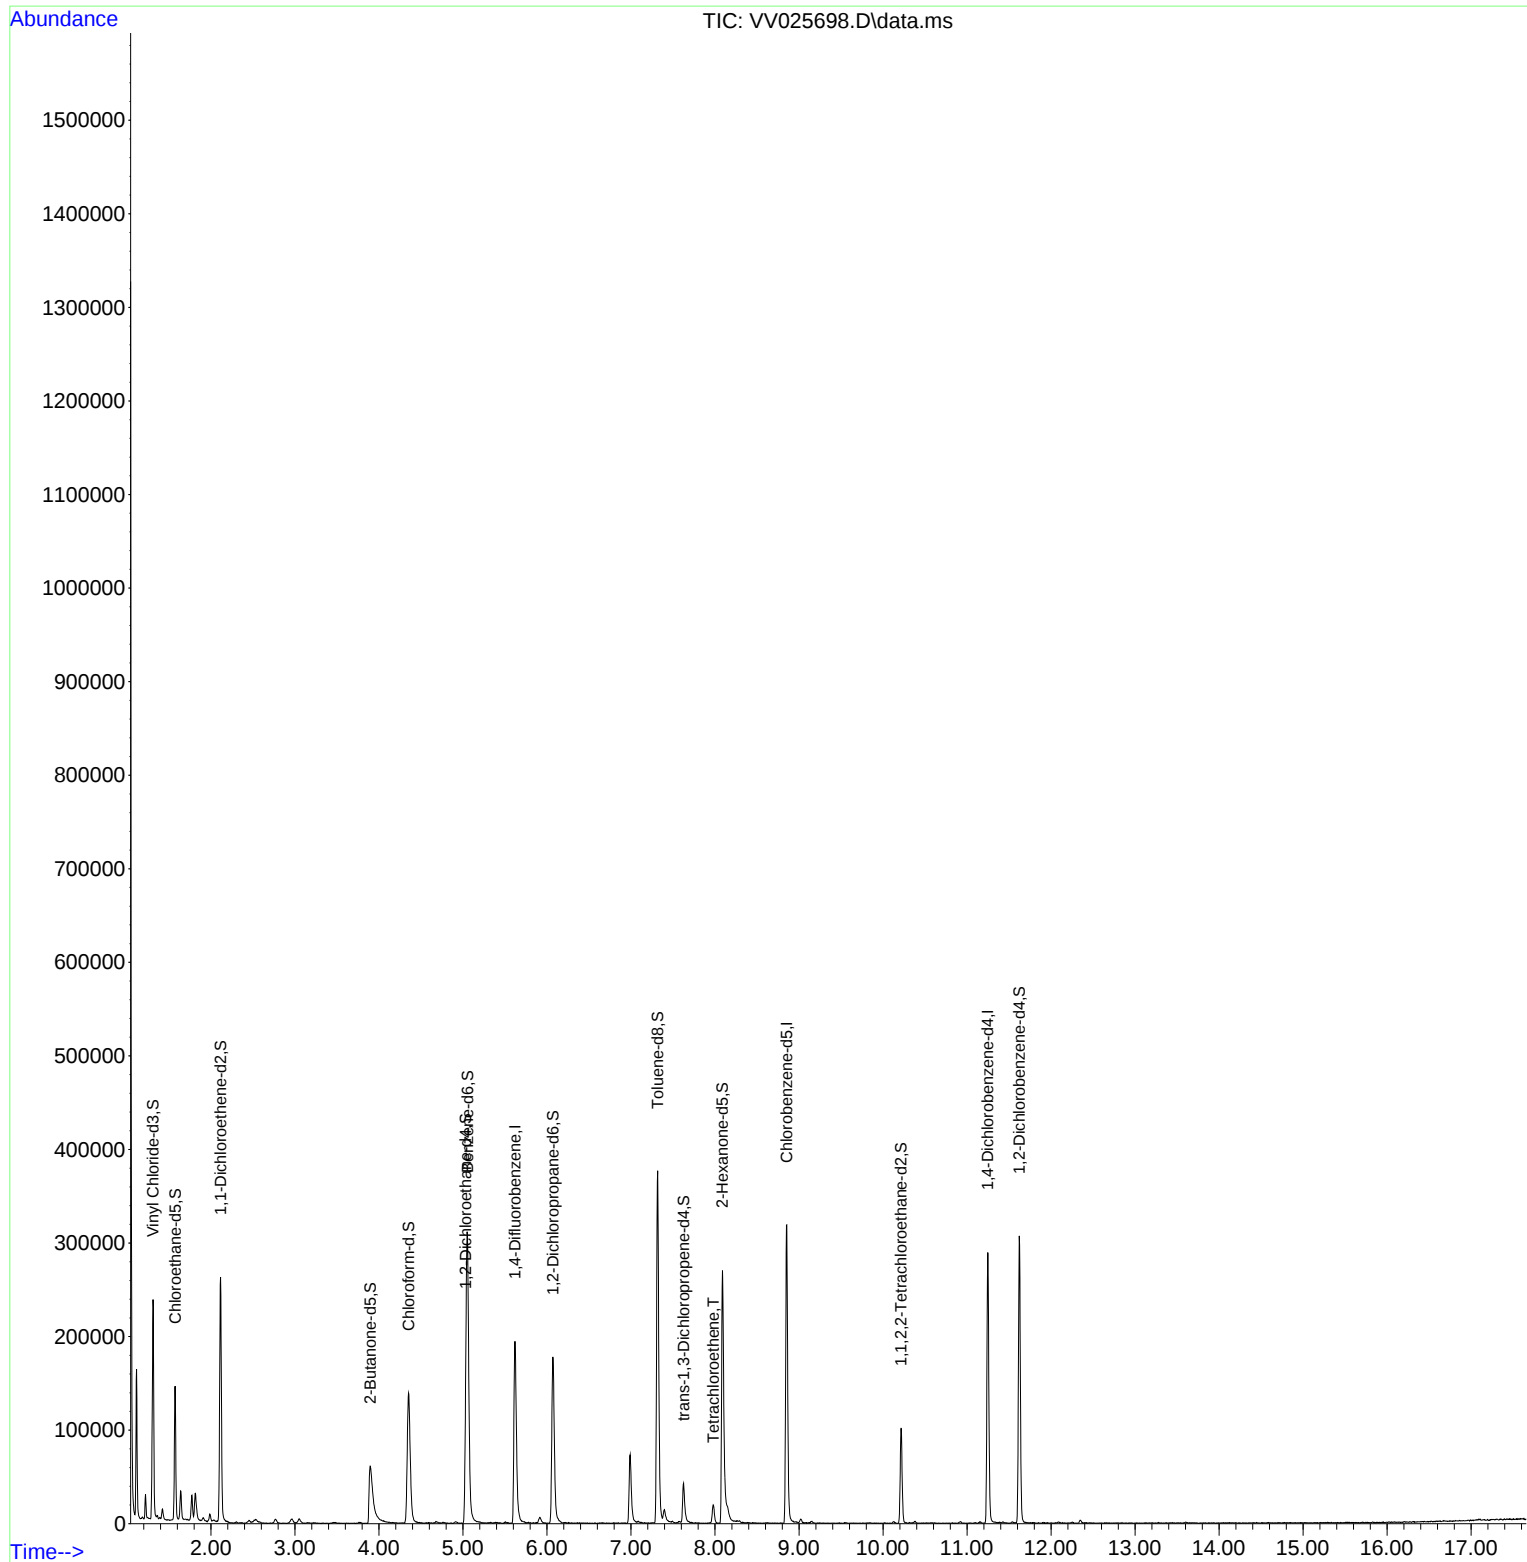

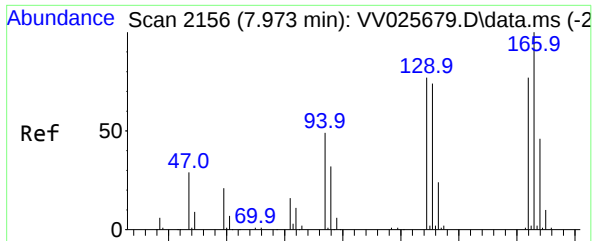

#47
 Tetrachloroethene
 Concen: 0.414 ug/L
 RT: 7.979 min Scan# 2156
 Delta R.T. 0.006 min
 Lab File: VV025698.D
 Acq: 22 Apr 2022 22:10

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6X2

Tgt Ion:164 Resp: 4433

Ion	Ratio	Lower	Upper
164	100		
129	96.0	66.8	124.2
131	88.8	66.4	123.4
166	122.4	91.7	170.3

