

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025680.D
 Acq On : 22 Apr 2022 14:27
 Operator : SY/MD
 Sample : VV0422WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	94	rBV	147970	152102	20.39%	2.553%
2	1.571	157	165	177	rBV	132627	150269	20.14%	2.522%
3	2.111	322	333	356	rVB	267388	392056	52.55%	6.580%
4	2.510	446	457	474	rBV2	16717	29985	4.02%	0.503%
5	3.043	614	623	637	rVB5	5092	10917	1.46%	0.183%
6	3.905	876	891	927	rBV	48127	201037	26.95%	3.374%
7	4.346	1011	1028	1056	rBV	127625	322162	43.18%	5.407%
8	5.047	1229	1246	1272	rBV2	299534	746043	100.00%	12.521%
9	5.616	1409	1423	1448	rBV	219547	452944	60.71%	7.602%
10	5.911	1503	1515	1528	rBV5	7198	15627	2.09%	0.262%
11	6.066	1550	1563	1589	rBV	168397	349585	46.86%	5.867%
12	6.985	1837	1849	1878	rBV2	71445	139491	18.70%	2.341%
13	7.313	1939	1951	1972	rBV	361092	636341	85.30%	10.680%
14	7.394	1972	1976	1990	rVB4	5845	11162	1.50%	0.187%
15	7.622	2038	2047	2066	rBV	39534	73960	9.91%	1.241%
16	8.088	2181	2192	2243	rBV	244435	491532	65.89%	8.250%
17	8.850	2417	2429	2451	rBV	353535	580346	77.79%	9.740%
18	10.214	2841	2853	2869	rBV2	93493	147716	19.80%	2.479%
19	11.246	3163	3174	3194	rBV	361893	558873	74.91%	9.380%
20	11.622	3277	3291	3309	rBV	308233	487503	65.35%	8.182%
21	13.506	3868	3877	3890	rBV	5785	8661	1.16%	0.145%




Sum of corrected areas: 5958312

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025680.D
Acq On : 22 Apr 2022 14:27
Operator : SY/MD
Sample : VV0422WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

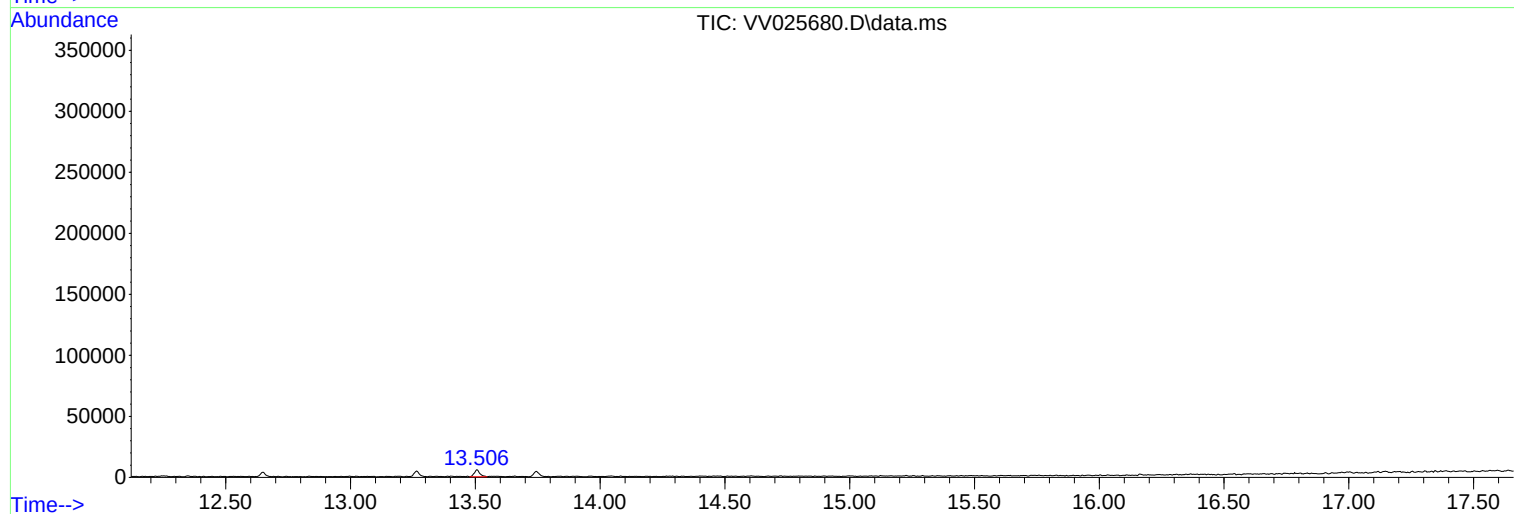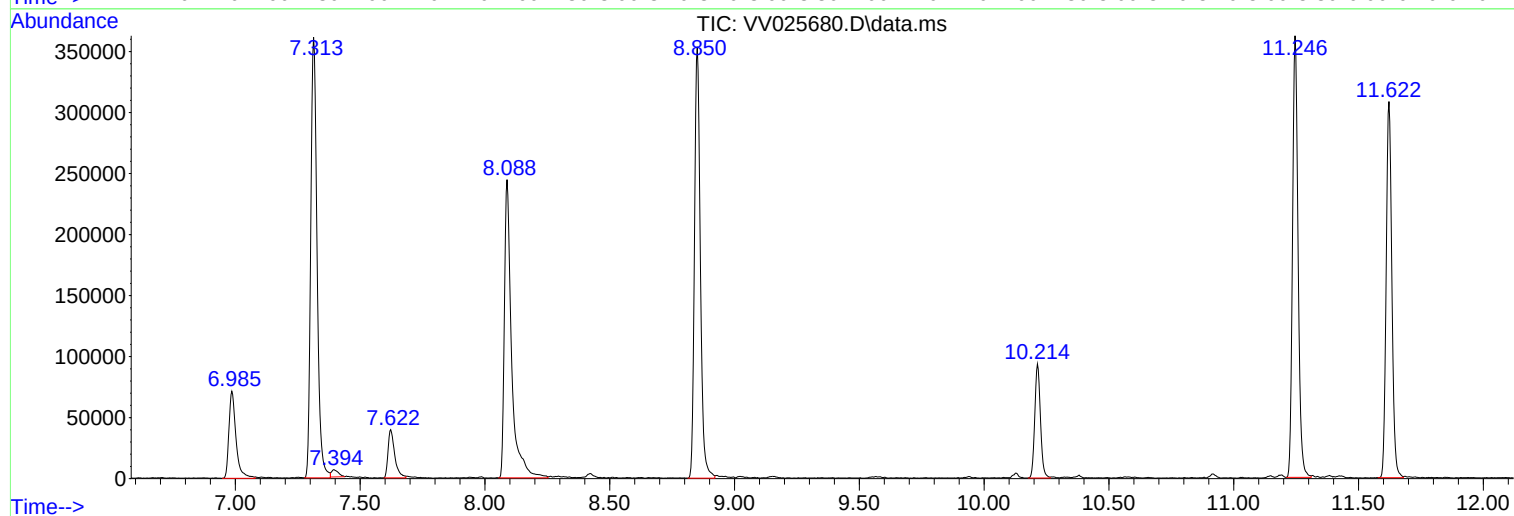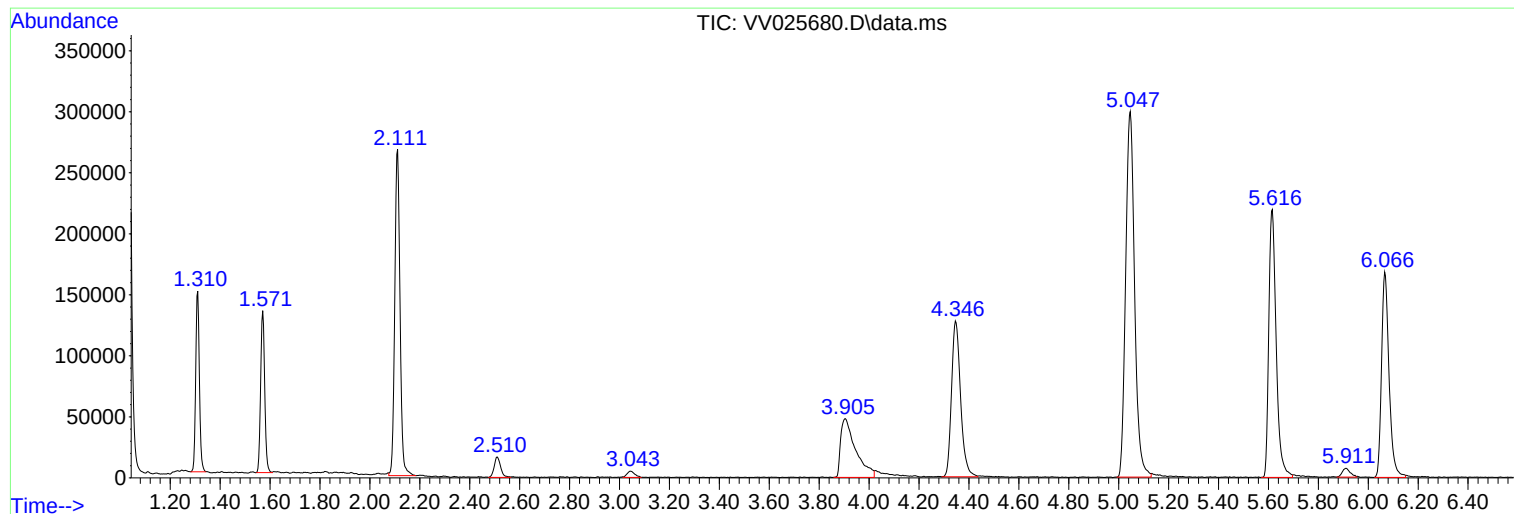

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025680.D
Acq On : 22 Apr 2022 14:27
Operator : SY/MD
Sample : VV0422WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025680.D
Acq On : 22 Apr 2022 14:27
Operator : SY/MD
Sample : VV0422WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------