

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025684.D
 Acq On : 22 Apr 2022 16:42
 Operator : SY/MD
 Sample : N2492-07DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	95	rVB	126363	126778	21.29%	2.679%
2	1.571	157	165	177	rBV	112593	125749	21.12%	2.658%
3	2.111	322	333	361	rVB	210920	313494	52.66%	6.625%
4	2.513	445	458	468	rBV2	6306	10560	1.77%	0.223%
5	3.899	877	889	925	rBV3	47779	170188	28.59%	3.597%
6	4.352	1016	1030	1056	rBV	104352	260946	43.83%	5.515%
7	5.050	1231	1247	1277	rBV2	237844	595352	100.00%	12.582%
8	5.619	1410	1424	1452	rBV	150967	314636	52.85%	6.649%
9	5.921	1506	1518	1532	rVB	7249	17173	2.88%	0.363%
10	6.072	1550	1565	1583	rBV	134244	277375	46.59%	5.862%
11	6.989	1840	1850	1874	rBV	55337	105625	17.74%	2.232%
12	7.317	1940	1952	1972	rBV	276951	493651	82.92%	10.433%
13	7.625	2039	2048	2068	rBV2	31805	57586	9.67%	1.217%
14	7.976	2146	2157	2174	rBV2	127935	221008	37.12%	4.671%
15	8.091	2182	2193	2236	rBV	190546	378999	63.66%	8.010%
16	8.853	2419	2430	2451	rBV	246095	408637	68.64%	8.636%
17	10.214	2843	2853	2866	rBV	75444	121122	20.34%	2.560%
18	11.249	3162	3175	3192	rBV	232873	361909	60.79%	7.648%
19	11.622	3278	3291	3312	rBV	236815	371047	62.32%	7.842%




Sum of corrected areas: 4731835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025684.D
Acq On : 22 Apr 2022 16:42
Operator : SY/MD
Sample : N2492-07DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

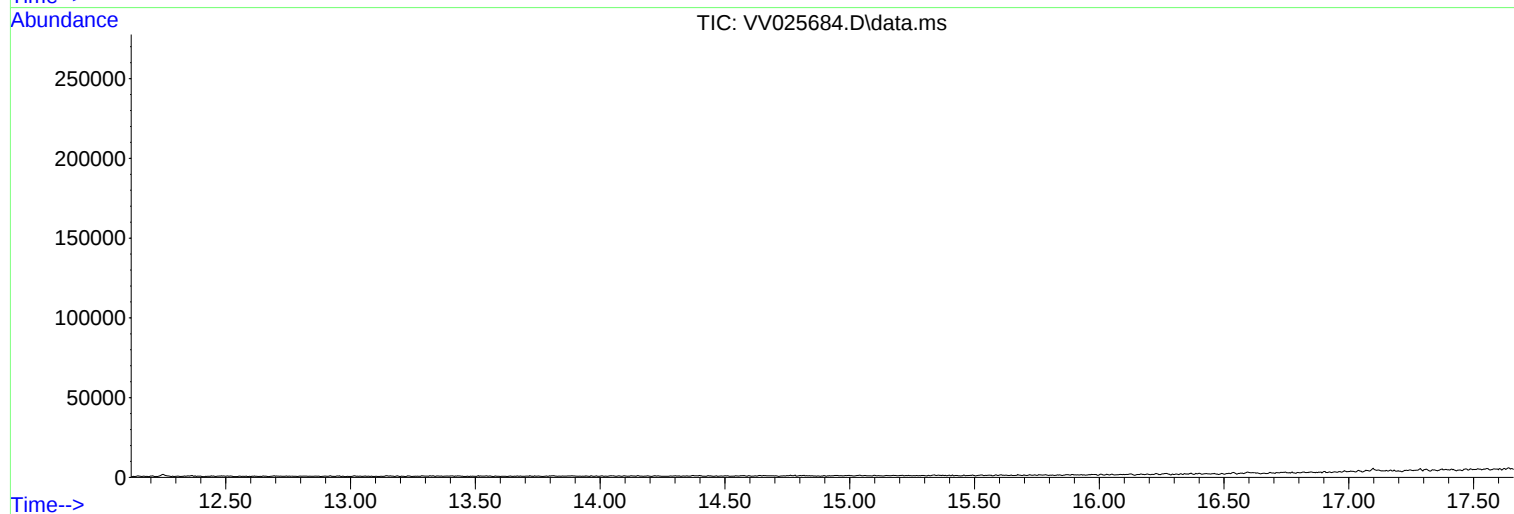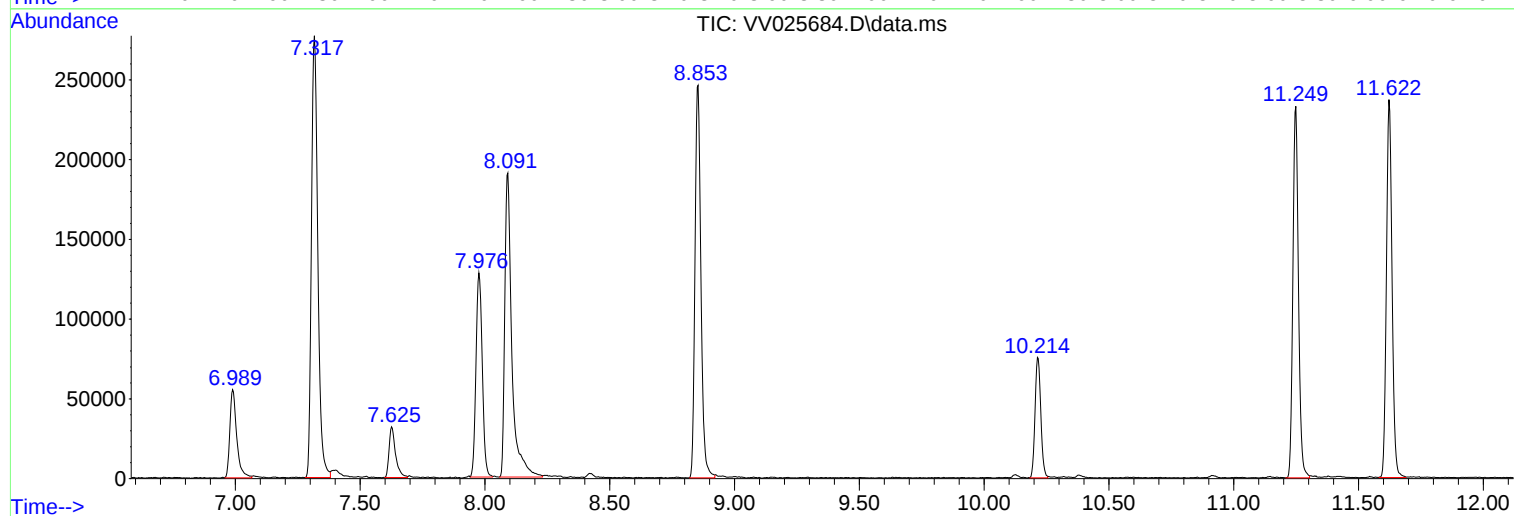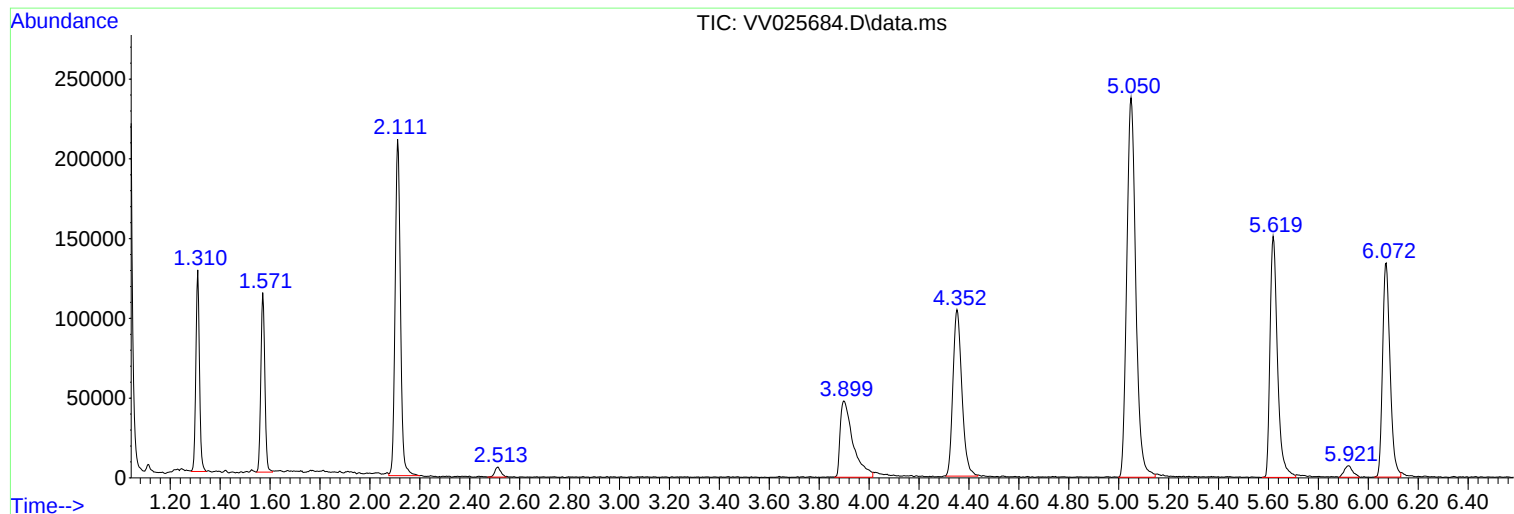

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025684.D
Acq On : 22 Apr 2022 16:42
Operator : SY/MD
Sample : N2492-07DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025684.D
Acq On : 22 Apr 2022 16:42
Operator : SY/MD
Sample : N2492-07DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc