

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025685.D
 Acq On : 22 Apr 2022 17:05
 Operator : SY/MD
 Sample : N2492-08DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rBV	111242	119150	20.69%	2.617%
2	1.571	157	165	174	rBV	111083	125097	21.73%	2.748%
3	2.111	322	333	352	rVB	202742	293427	50.96%	6.445%
4	2.510	449	457	473	rVB2	6103	10022	1.74%	0.220%
5	3.899	877	889	924	rBV	47115	164607	28.59%	3.615%
6	4.352	1014	1030	1052	rBV	103723	259067	44.99%	5.690%
7	5.050	1230	1247	1276	rBV2	230419	575780	100.00%	12.646%
8	5.619	1411	1424	1451	rBV	147656	303845	52.77%	6.674%
9	5.918	1504	1517	1530	rBV10	5000	11459	1.99%	0.252%
10	6.069	1552	1564	1594	rBV	130669	271754	47.20%	5.969%
11	6.989	1837	1850	1873	rBV	52962	102971	17.88%	2.262%
12	7.317	1941	1952	1972	rBV	265564	471517	81.89%	10.356%
13	7.625	2039	2048	2062	rBV2	30774	54163	9.41%	1.190%
14	7.976	2145	2157	2175	rBV	131186	221719	38.51%	4.870%
15	8.088	2183	2192	2229	rBV	187514	371124	64.46%	8.151%
16	8.850	2418	2429	2450	rBV	231903	387221	67.25%	8.505%
17	10.214	2841	2853	2870	rBV	73652	117981	20.49%	2.591%
18	11.249	3164	3175	3194	rBV	220444	340426	59.12%	7.477%
19	11.622	3279	3291	3314	rBV	223862	351582	61.06%	7.722%




Sum of corrected areas: 4552912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025685.D
Acq On : 22 Apr 2022 17:05
Operator : SY/MD
Sample : N2492-08DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

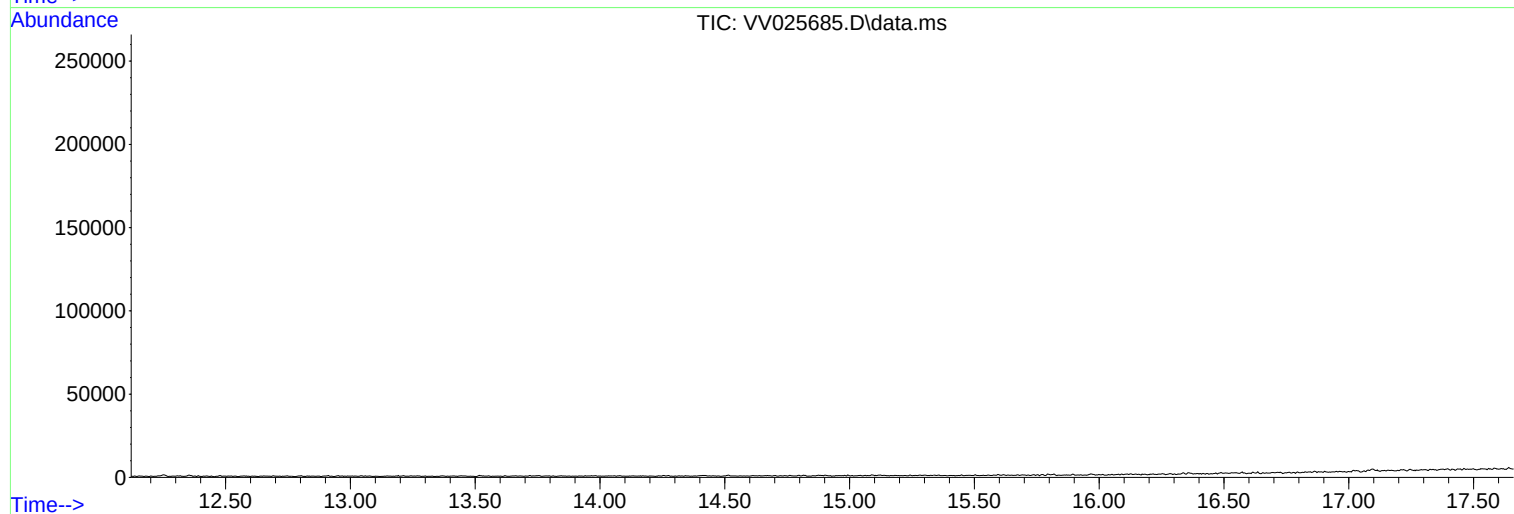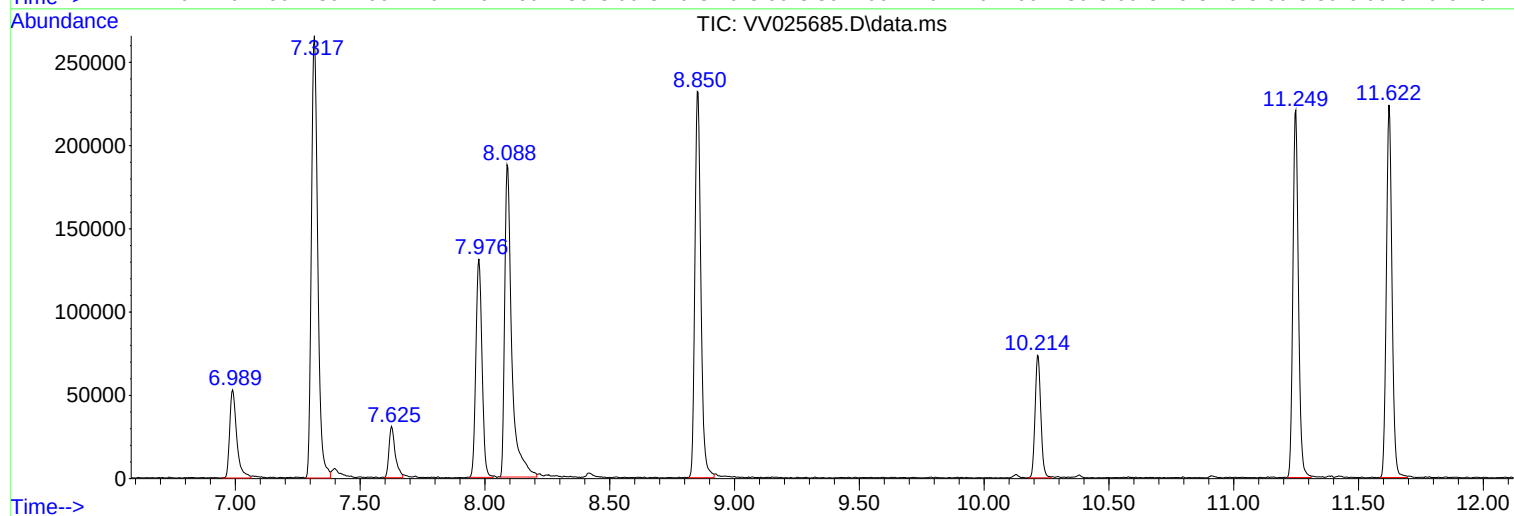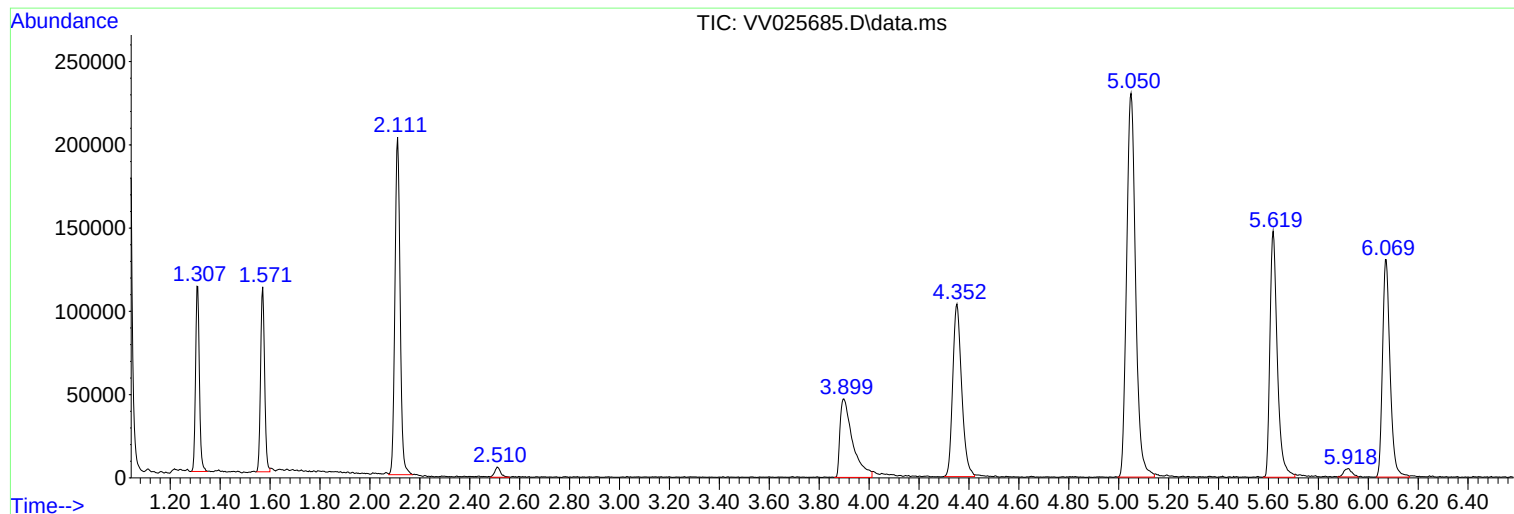

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025685.D
Acq On : 22 Apr 2022 17:05
Operator : SY/MD
Sample : N2492-08DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025685.D
Acq On : 22 Apr 2022 17:05
Operator : SY/MD
Sample : N2492-08DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------