

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025686.D
 Acq On : 22 Apr 2022 17:29
 Operator : SY/MD
 Sample : N2492-09DL 200X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	98	rVB	126292	124189	20.63%	2.587%
2	1.571	157	165	177	rBV	110697	124877	20.74%	2.601%
3	2.111	323	333	360	rVB	212484	310201	51.52%	6.462%
4	2.513	449	458	472	rVB3	6480	11137	1.85%	0.232%
5	3.902	879	890	911	rBV	48672	159833	26.55%	3.330%
6	4.352	1014	1030	1060	rBV2	106852	271174	45.04%	5.649%
7	5.050	1231	1247	1272	rBV2	241393	602064	100.00%	12.542%
8	5.619	1410	1424	1451	rBV	151189	312047	51.83%	6.500%
9	5.912	1507	1515	1531	rBV8	5195	12203	2.03%	0.254%
10	6.072	1552	1565	1596	rBV	136108	284048	47.18%	5.917%
11	6.989	1839	1850	1869	rBV2	55673	106044	17.61%	2.209%
12	7.317	1941	1952	1973	rBV	275288	489239	81.26%	10.192%
13	7.625	2036	2048	2071	rBV	32128	61633	10.24%	1.284%
14	7.976	2146	2157	2177	rBV	162135	274465	45.59%	5.718%
15	8.092	2183	2193	2231	rBV	197642	399156	66.30%	8.315%
16	8.423	2288	2296	2311	rVB5	3821	6896	1.15%	0.144%
17	8.854	2417	2430	2458	rBV	241509	406822	67.57%	8.475%
18	10.214	2839	2853	2871	rBV	79651	123784	20.56%	2.579%
19	11.249	3163	3175	3193	rBV	225393	353966	58.79%	7.374%
20	11.622	3280	3291	3310	rBV	230939	366613	60.89%	7.637%




Sum of corrected areas: 4800391

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025686.D
Acq On : 22 Apr 2022 17:29
Operator : SY/MD
Sample : N2492-09DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

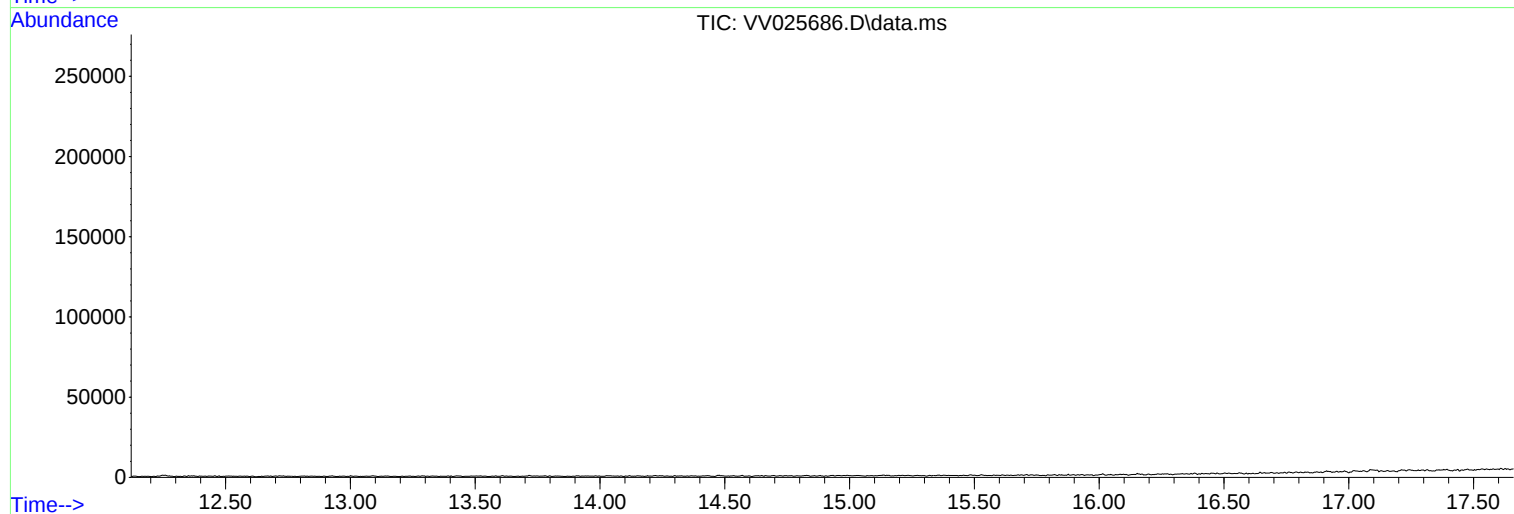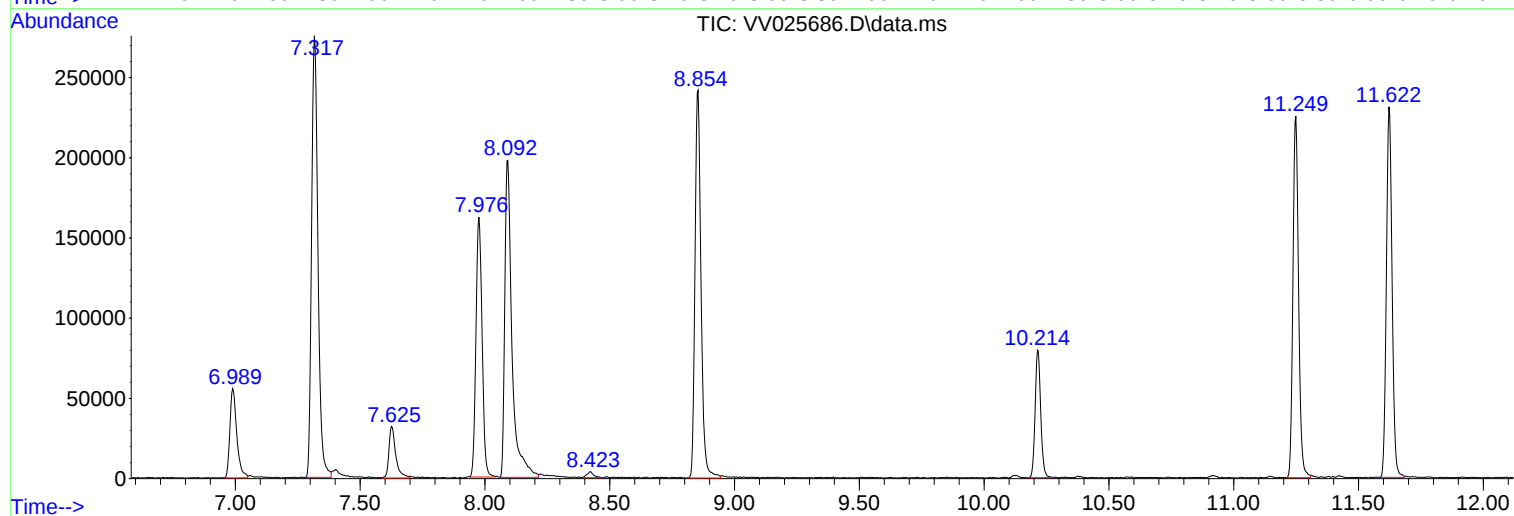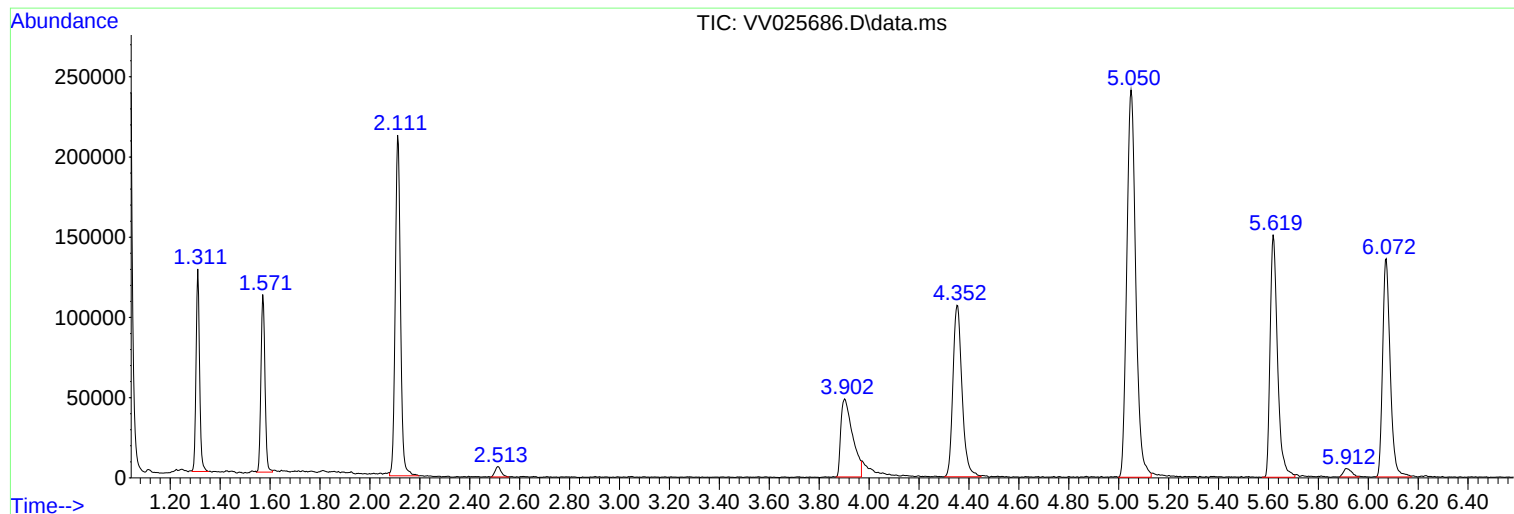

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025686.D
Acq On : 22 Apr 2022 17:29
Operator : SY/MD
Sample : N2492-09DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025686.D
Acq On : 22 Apr 2022 17:29
Operator : SY/MD
Sample : N2492-09DL 200X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------