

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025687.D
 Acq On : 22 Apr 2022 17:52
 Operator : SY/MD
 Sample : N2492-04DL 500X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6T6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	97	rVB	124862	127846	21.30%	2.786%
2	1.571	157	165	178	rBV	112070	126546	21.09%	2.757%
3	2.111	322	333	349	rVB	215171	310206	51.69%	6.759%
4	2.513	449	458	468	rBV4	4519	7502	1.25%	0.163%
5	3.902	877	890	935	rBV3	46534	180734	30.12%	3.938%
6	4.352	1012	1030	1056	rBV	105365	269993	44.99%	5.883%
7	5.050	1231	1247	1275	rBV2	240201	600081	100.00%	13.076%
8	5.619	1413	1424	1442	rBV2	143035	295067	49.17%	6.429%
9	5.918	1507	1517	1528	rBV10	5355	11486	1.91%	0.250%
10	6.072	1552	1565	1586	rBV	133659	280508	46.75%	6.112%
11	6.989	1839	1850	1877	rBV	53596	106748	17.79%	2.326%
12	7.317	1941	1952	1971	rBV	285914	501682	83.60%	10.931%
13	7.625	2040	2048	2063	rBV2	29982	55953	9.32%	1.219%
14	7.976	2146	2157	2174	rVB	66059	114702	19.11%	2.499%
15	8.091	2183	2193	2226	rBV	186652	376550	62.75%	8.205%
16	8.423	2287	2296	2305	rVB5	4309	7150	1.19%	0.156%
17	8.853	2419	2430	2447	rBV	229408	380426	63.40%	8.289%
18	10.217	2842	2854	2872	rBV	76734	123331	20.55%	2.687%
19	11.249	3164	3175	3200	rBV	217136	338387	56.39%	7.373%
20	11.622	3280	3291	3308	rBV	236834	374441	62.40%	8.159%




Sum of corrected areas: 4589339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025687.D
Acq On : 22 Apr 2022 17:52
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

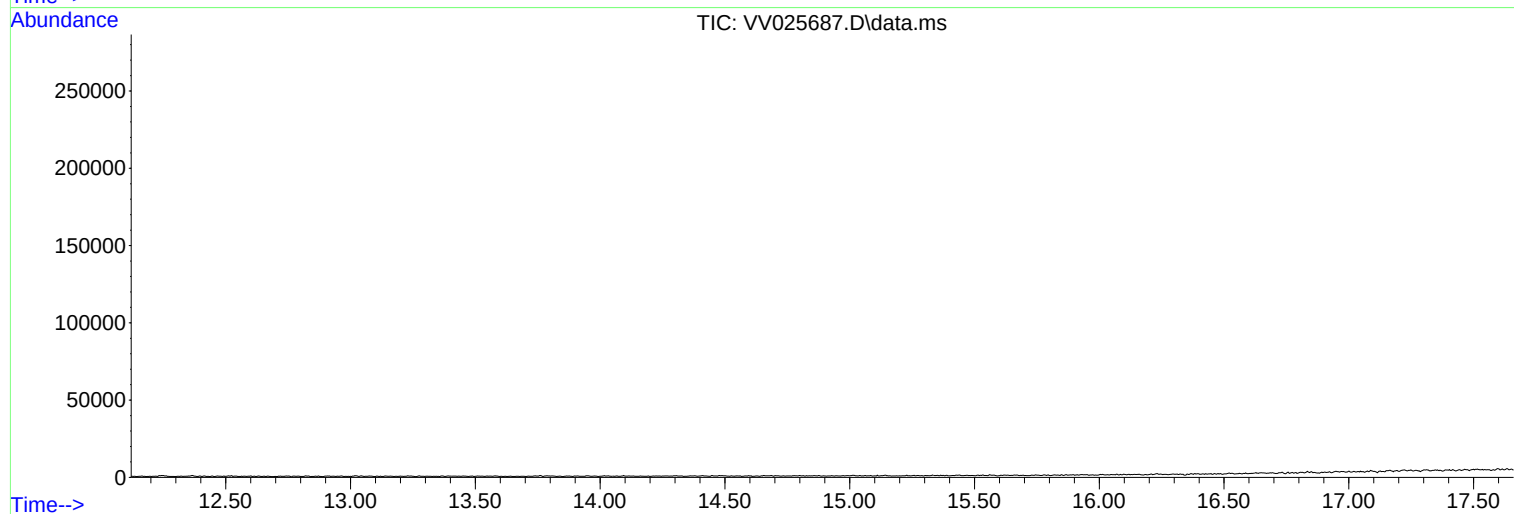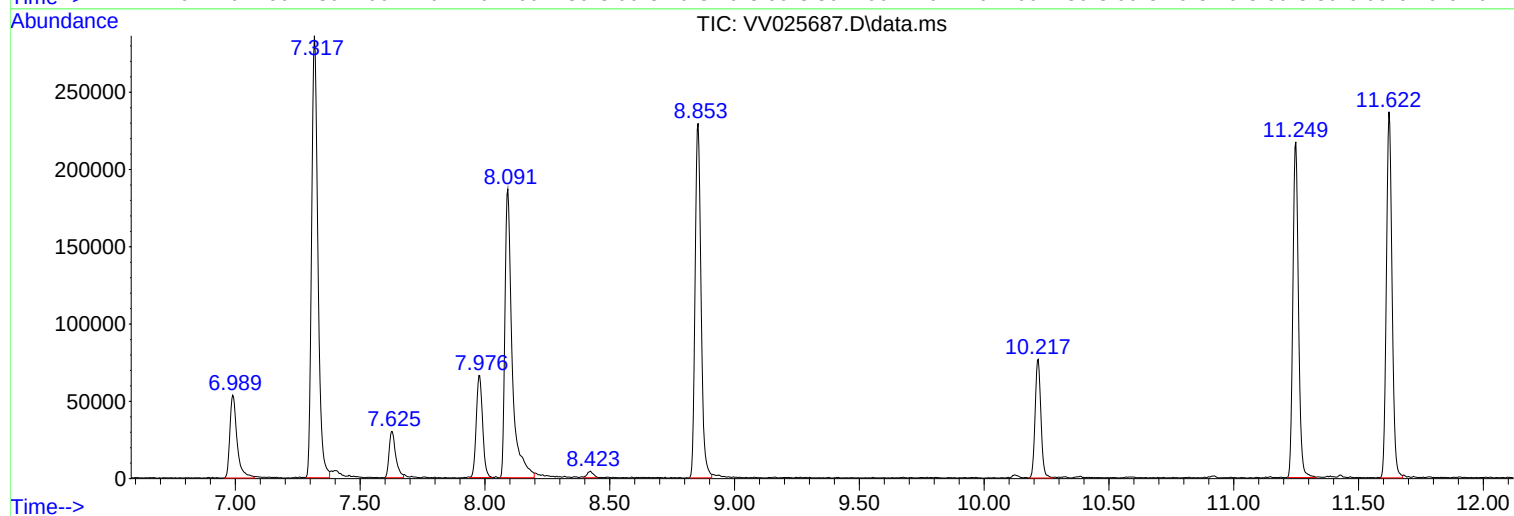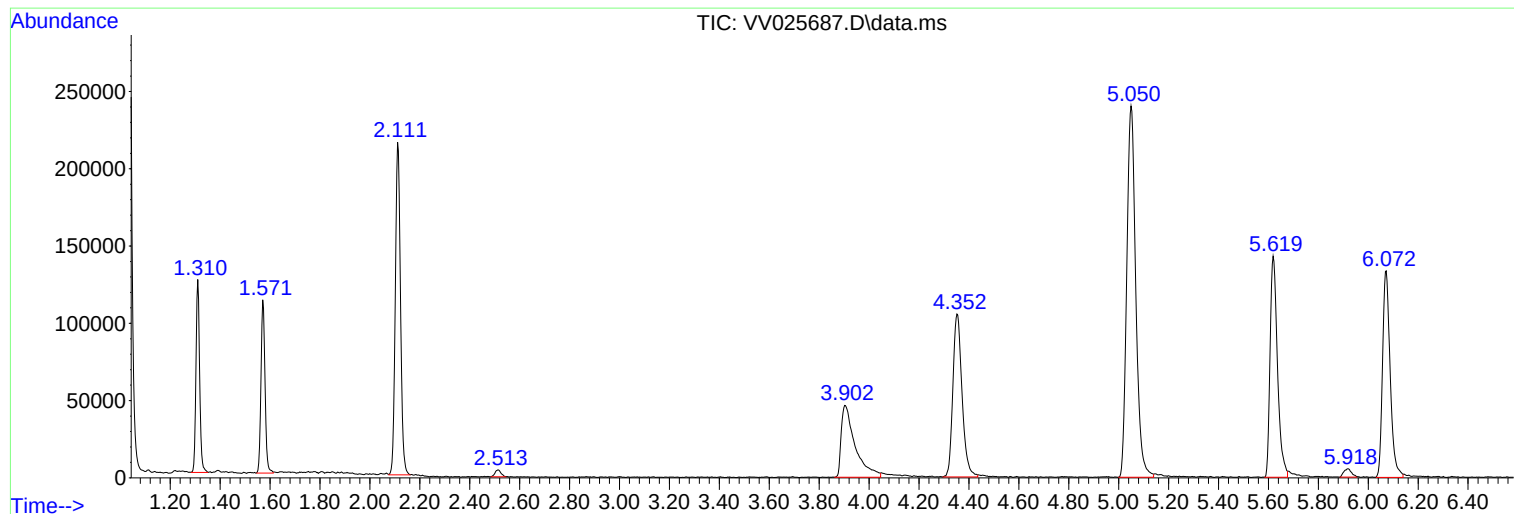

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025687.D
Acq On : 22 Apr 2022 17:52
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025687.D
Acq On : 22 Apr 2022 17:52
Operator : SY/MD
Sample : N2492-04DL 500X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6T6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------