

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025689.D
 Acq On : 22 Apr 2022 18:39
 Operator : SY/MD
 Sample : N2530-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Z0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	77	84	100	rVB	122236	121977	20.66%	2.772%
2	1.571	158	165	179	rVB	109851	123245	20.88%	2.801%
3	2.111	321	333	356	rVB	196826	290408	49.19%	6.599%
4	2.513	447	458	473	rVB2	16888	29622	5.02%	0.673%
5	3.908	881	892	929	rBV2	38288	157697	26.71%	3.583%
6	4.352	1013	1030	1060	rBV	105350	266766	45.19%	6.062%
7	5.050	1231	1247	1277	rBV2	235959	590338	100.00%	13.415%
8	5.619	1413	1424	1445	rBV	141960	292914	49.62%	6.656%
9	5.912	1507	1515	1533	rVB7	6303	13799	2.34%	0.314%
10	6.072	1550	1565	1586	rBV2	137225	282578	47.87%	6.421%
11	6.989	1840	1850	1869	rBV2	55001	103548	17.54%	2.353%
12	7.317	1941	1952	1968	rBV	248448	438571	74.29%	9.966%
13	7.394	1968	1976	1992	rVB	24098	49243	8.34%	1.119%
14	7.625	2038	2048	2072	rBV2	30833	57738	9.78%	1.312%
15	8.092	2182	2193	2231	rBV	196831	418136	70.83%	9.502%
16	8.854	2419	2430	2454	rBV	226389	373966	63.35%	8.498%
17	9.146	2511	2521	2534	rBV3	8005	13836	2.34%	0.314%
18	10.214	2842	2853	2868	rBV	77371	123720	20.96%	2.811%
19	10.384	2897	2906	2913	rBV4	4169	6302	1.07%	0.143%
20	11.249	3163	3175	3193	rBV	204980	320462	54.28%	7.282%
21	11.622	3279	3291	3310	rBV	206249	325831	55.19%	7.404%




Sum of corrected areas: 4400697

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025689.D
Acq On : 22 Apr 2022 18:39
Operator : SY/MD
Sample : N2530-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

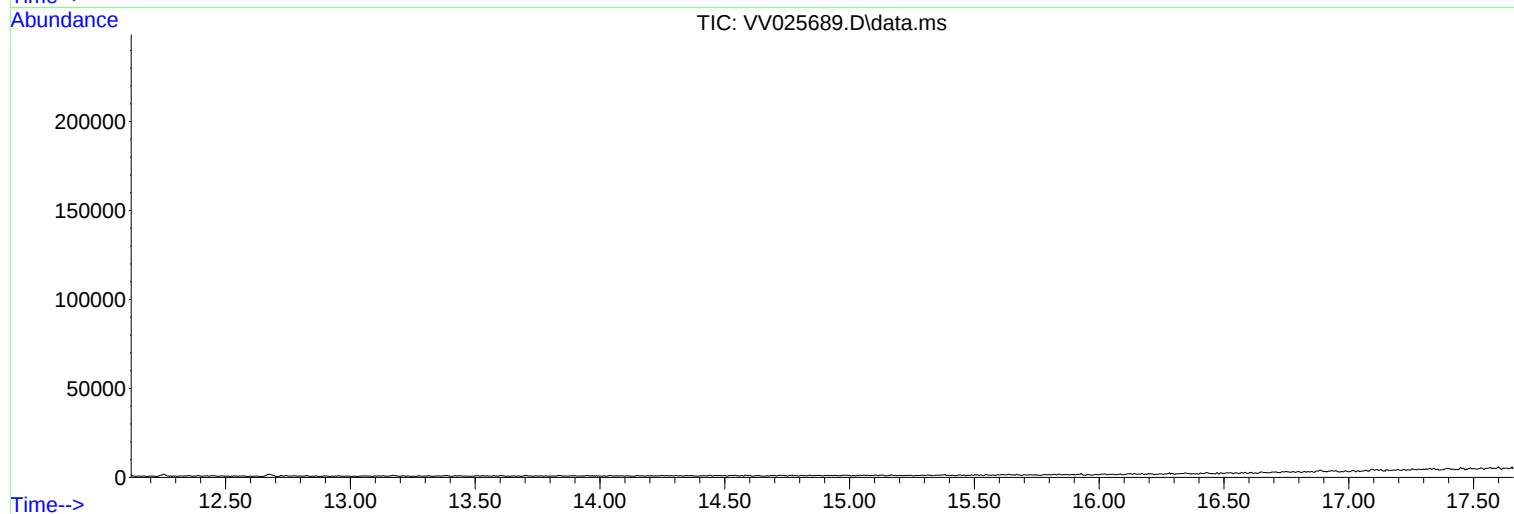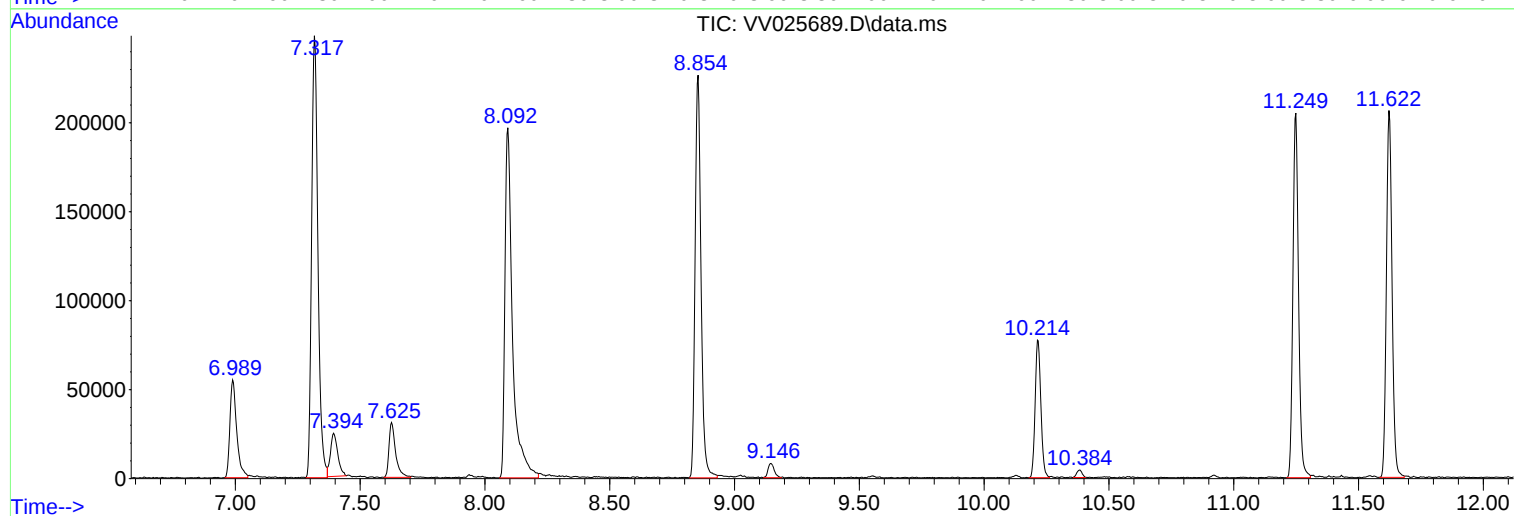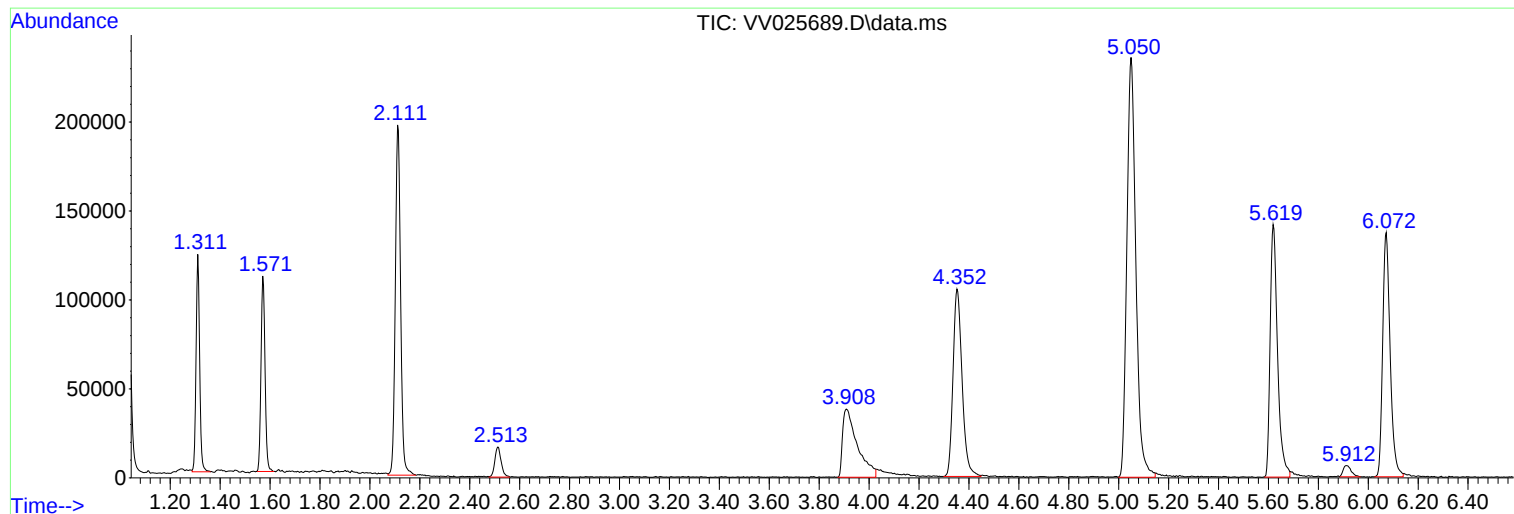

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025689.D
Acq On : 22 Apr 2022 18:39
Operator : SY/MD
Sample : N2530-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025689.D
Acq On : 22 Apr 2022 18:39
Operator : SY/MD
Sample : N2530-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc