

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
 Data File : VV025693.D
 Acq On : 22 Apr 2022 20:13
 Operator : SY/MD
 Sample : N2492-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6W7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	34	rVB2	7960	9108	1.01%	0.178%
2	1.310	77	84	95	rBV	113757	116905	12.98%	2.290%
3	1.571	158	165	178	rBV	100075	113972	12.66%	2.233%
4	2.114	323	334	356	rVB	191884	283325	31.46%	5.550%
5	3.899	880	889	916	rBV	41545	134686	14.96%	2.638%
6	4.352	1015	1030	1058	rBV2	98856	249662	27.72%	4.891%
7	5.050	1229	1247	1279	rBV3	222977	557976	61.96%	10.930%
8	5.619	1413	1424	1448	rBV	139693	290427	32.25%	5.689%
9	5.915	1505	1516	1536	rBV	6916	16103	1.79%	0.315%
10	6.072	1551	1565	1593	rBV	128343	264717	29.39%	5.186%
11	6.989	1841	1850	1877	rBV2	52615	100497	11.16%	1.969%
12	7.317	1940	1952	1971	rBV	258598	457426	50.79%	8.961%
13	7.400	1971	1978	1990	rVB3	5768	12441	1.38%	0.244%
14	7.625	2040	2048	2068	rBV	28659	52812	5.86%	1.035%
15	7.976	2145	2157	2181	rBV	541908	900592	100.00%	17.642%
16	8.092	2183	2193	2226	rVV	178779	356556	39.59%	6.985%
17	8.854	2418	2430	2456	rBV	235287	390246	43.33%	7.645%
18	10.214	2842	2853	2868	rBV	71623	114469	12.71%	2.242%
19	11.249	3164	3175	3195	rBV	219577	340667	37.83%	6.673%
20	11.622	3278	3291	3311	rBV	222730	342324	38.01%	6.706%




Sum of corrected areas: 5104911

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025693.D
Acq On : 22 Apr 2022 20:13
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

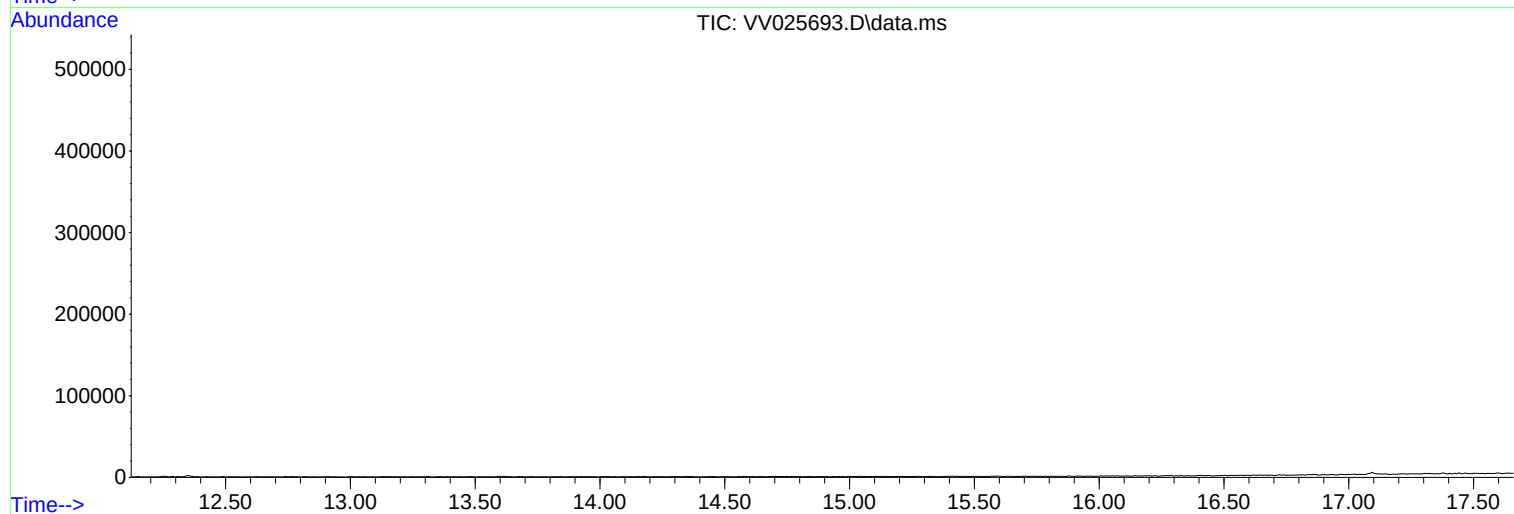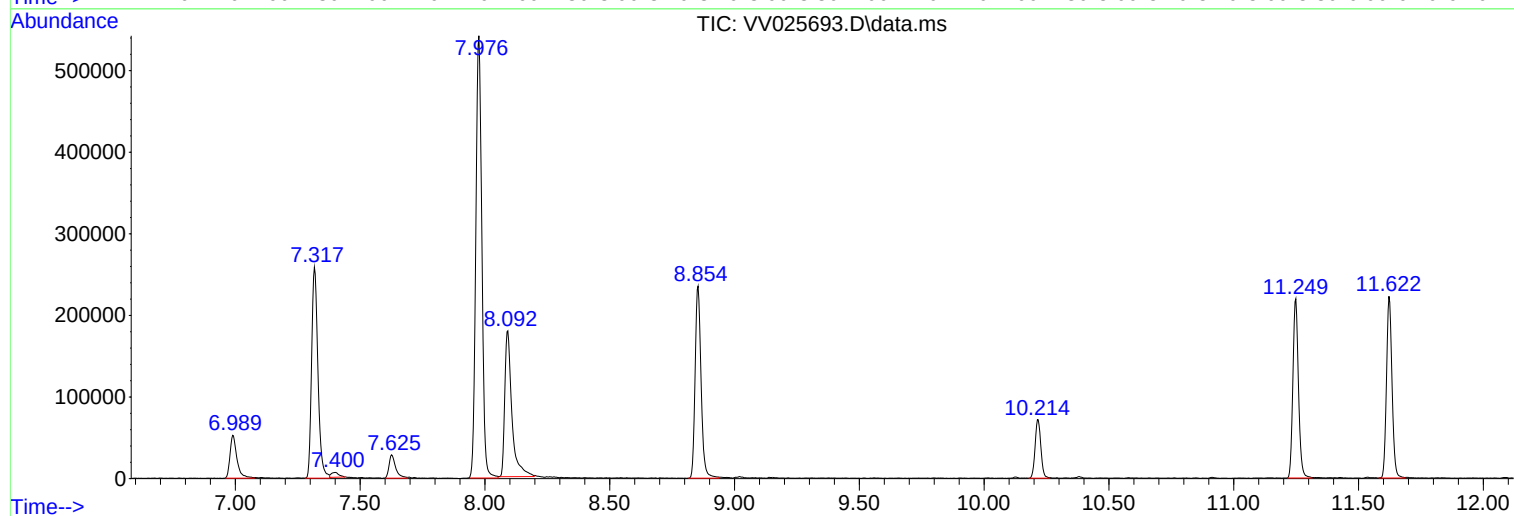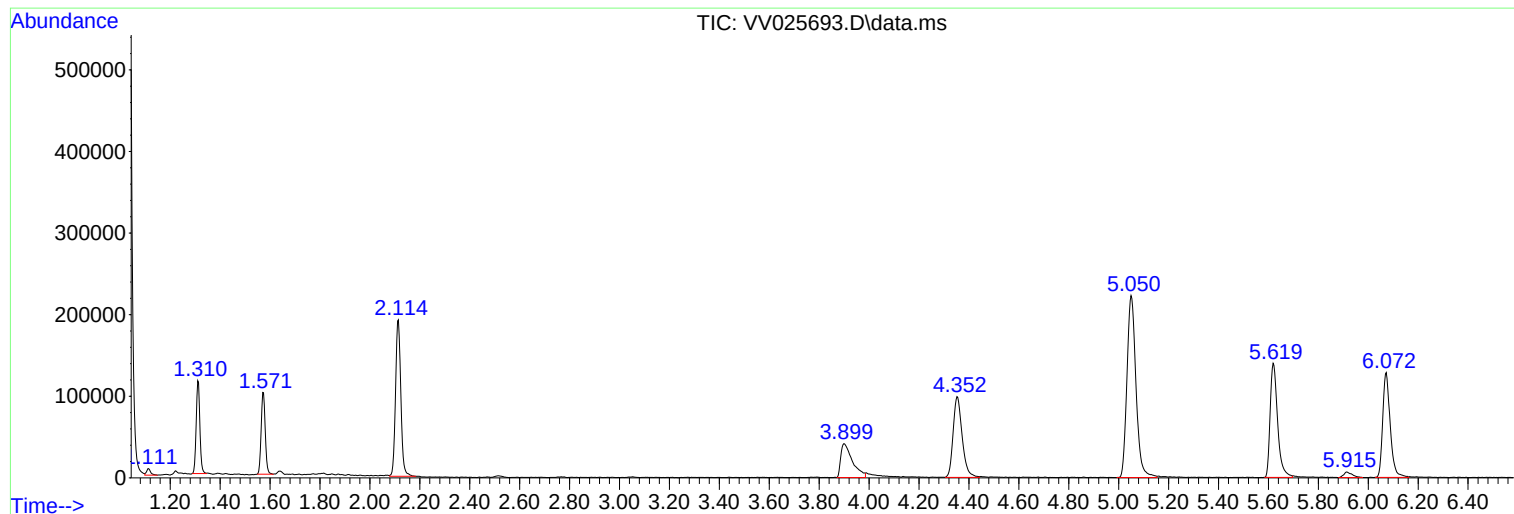

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025693.D
Acq On : 22 Apr 2022 20:13
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042222\
Data File : VV025693.D
Acq On : 22 Apr 2022 20:13
Operator : SY/MD
Sample : N2492-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6W7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc