

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042424\
 Data File : VW035386.D
 Acq On : 24 Apr 2024 14:48
 Operator : SY/MD
 Sample : P2238-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D16

Quant Time: Apr 25 02:00:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 01:57:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	394207	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	401361	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	188748	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	163514	42.950	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.900%
7) Chloroethane-d5	1.532	69	138963	42.025	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	84.040%
11) 1,1-Dichloroethene-d2	2.060	65	70755	42.398	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.800%
21) 2-Butanone-d5	3.796	46	203033	89.921	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.920%
24) Chloroform-d	4.246	84	312986	48.897	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	4.940	65	194267	47.803	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.600%
32) Benzene-d6	4.960	84	613947	45.539	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.080%
36) 1,2-Dichloropropane-d6	5.989	67	201428	47.050	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.100%
41) Toluene-d8	7.243	98	522700	43.050	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.100%
43) trans-1,3-Dichloroprop...	7.551	79	82883	39.823	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.640%
47) 2-Hexanone-d5	8.024	63	108262	66.885	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	66.880%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	282527	47.923	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.840%
66) 1,2-Dichlorobenzene-d4	11.558	152	218628	51.590	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.180%
Target Compounds						
13) Acetone	2.130	43	10683	5.154	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035386.D
Acq On : 24 Apr 2024 14:48
Operator : SY/MD
Sample : P2238-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D16

Quant Time: Apr 25 02:00:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 25 01:57:41 2024
Response via : Initial Calibration

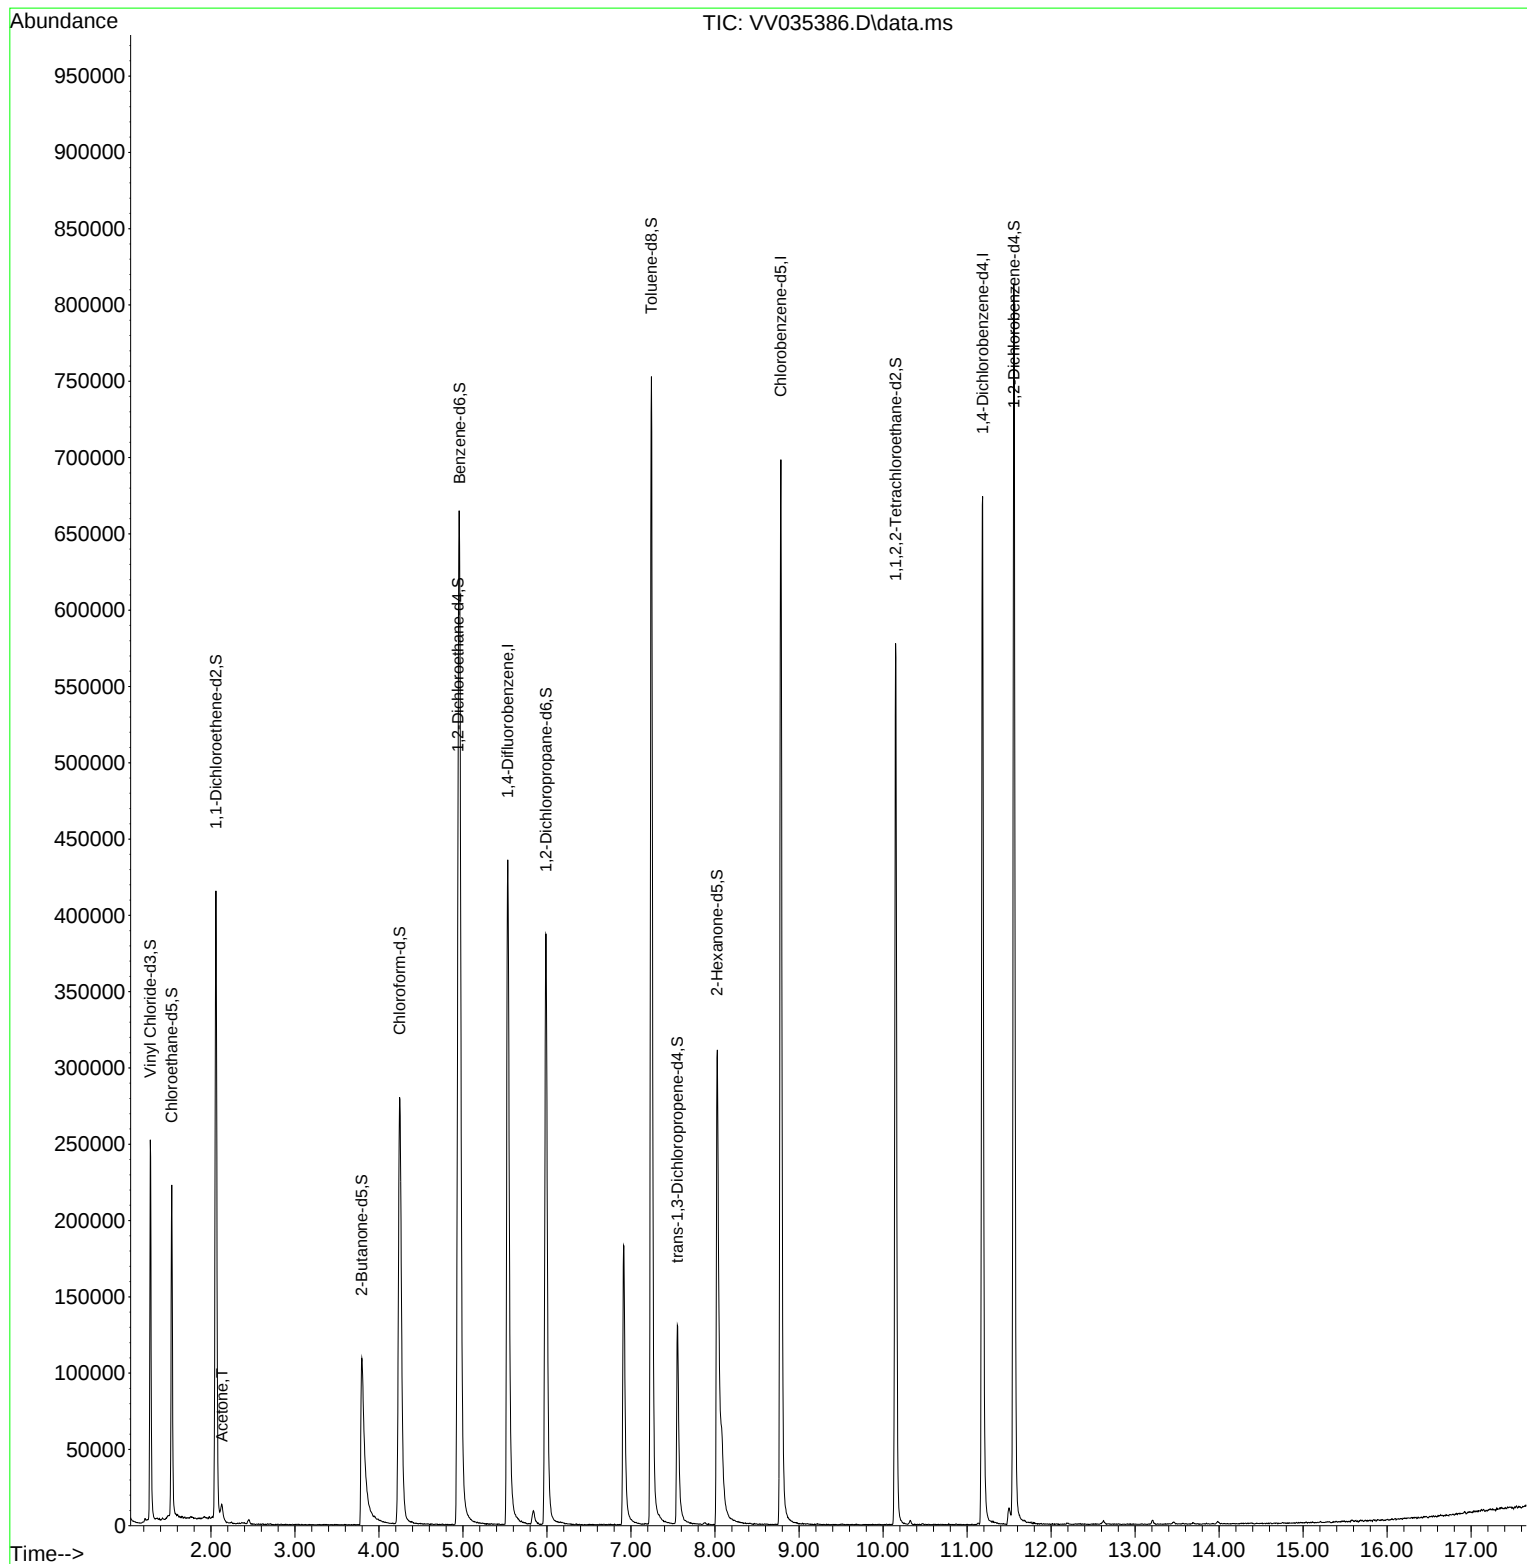

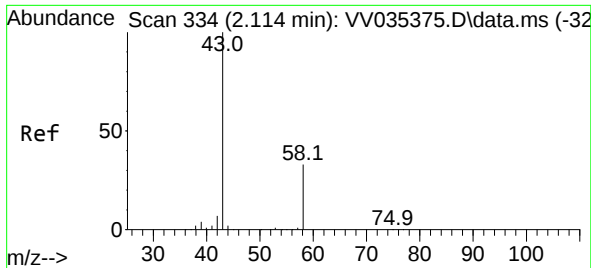

#13
 Acetone
 Concen: 5.154 ug/L
 RT: 2.130 min Scan# 31
 Delta R.T. 0.016 min
 Lab File: VV035386.D
 Acq: 24 Apr 2024 14:48

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D16

Tgt Ion: 43 Resp: 10683
 Ion Ratio Lower Upper
 43 100
 58 35.1 0.0 66.0

