

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035396.D
 Acq On : 24 Apr 2024 18:39
 Operator : SY/MD
 Sample : P2182-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0R94

Quant Time: Apr 25 02:02:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 25 01:57:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	389465	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	392856	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	179229	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	155297	41.288	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.580%		
7) Chloroethane-d5	1.532	69	134407	41.142	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.280%		
11) 1,1-Dichloroethene-d2	2.060	65	66266	40.191	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.380%		
21) 2-Butanone-d5	3.793	46	188497	84.500	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.500%		
24) Chloroform-d	4.249	84	307284	48.591	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.180%		
26) 1,2-Dichloroethane-d4	4.941	65	190761	47.512	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.020%		
32) Benzene-d6	4.960	84	594033	45.015	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.040%		
36) 1,2-Dichloropropane-d6	5.986	67	196024	46.779	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.560%		
41) Toluene-d8	7.243	98	503289	42.349	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.700%		
43) trans-1,3-Dichloroprop...	7.555	79	81713	40.111	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.220%		
47) 2-Hexanone-d5	8.024	63	105609	66.658	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	66.660%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	278968	48.343	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.680%		
66) 1,2-Dichlorobenzene-d4	11.558	152	209272	52.005	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	104.000%		
Target Compounds					Qvalue	
13) Acetone	2.121	43	17610	8.599	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035396.D
Acq On : 24 Apr 2024 18:39
Operator : SY/MD
Sample : P2182-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0R94

Quant Time: Apr 25 02:02:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 25 01:57:41 2024
Response via : Initial Calibration

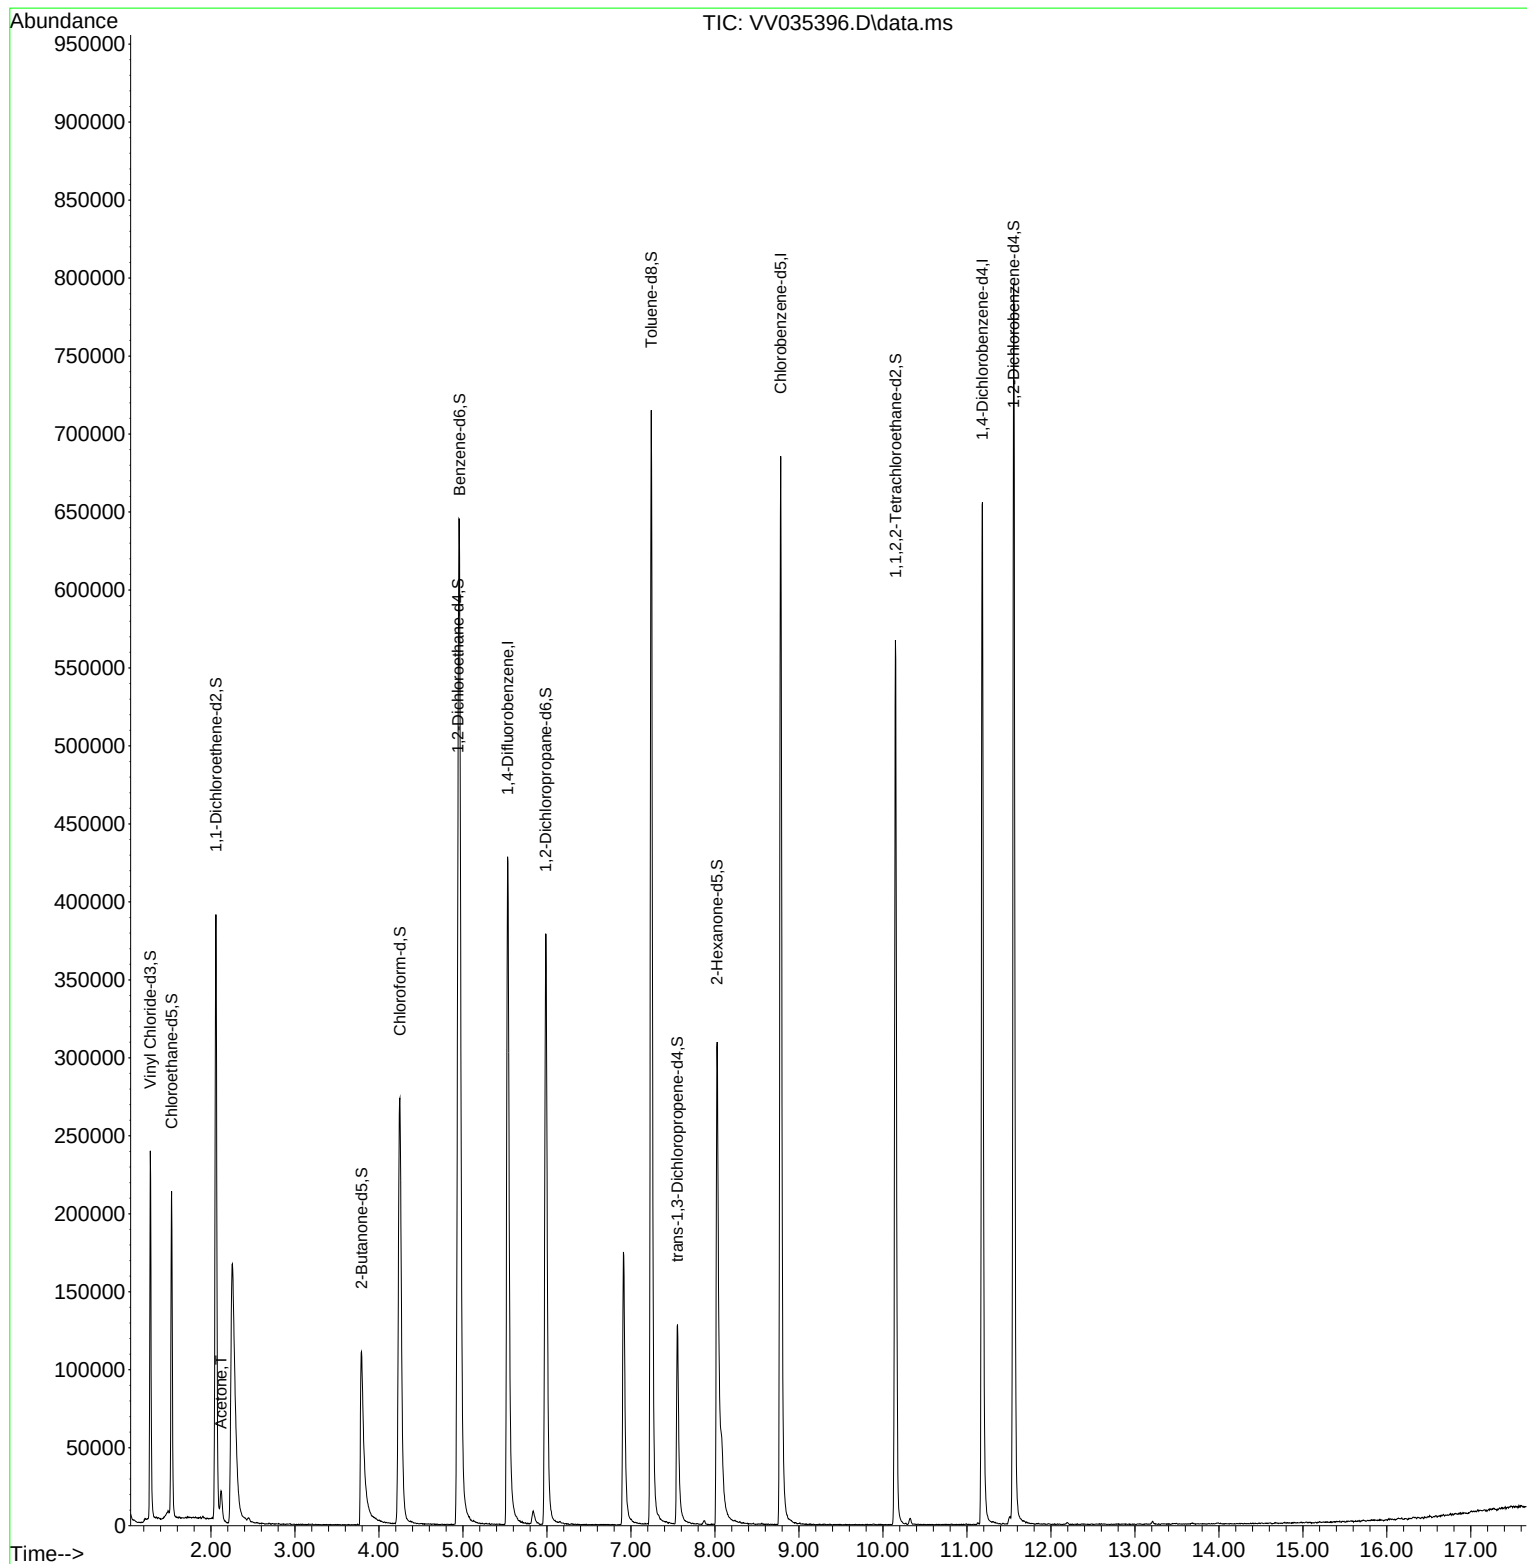

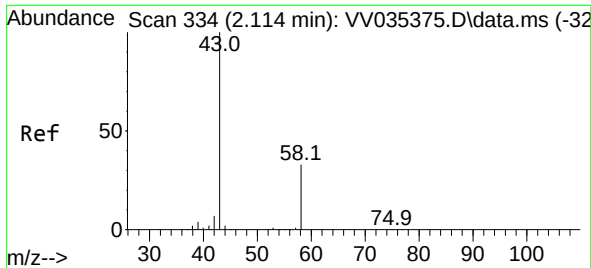

#13

Acetone

Concen: 8.599 ug/L

RT: 2.121 min Scan# 31

Delta R.T. 0.007 min

Lab File: VV035396.D

Acq: 24 Apr 2024 18:39

Instrument :

MSVOA_V

ClientSampleId :

MC0R94

Tgt Ion: 43 Resp: 17610

Ion Ratio Lower Upper

43 100

58 36.6 0.0 66.0

