

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035377.D
 Acq On : 24 Apr 2024 11:19
 Operator : SY/MD
 Sample : P2234-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	262812	284807	15.09%	2.089%
2	1.532	146	153	173	rVB	226645	268819	14.24%	1.972%
3	2.060	307	317	333	rBV	438402	630362	33.40%	4.623%
4	2.629	491	494	496	rBV2	173	125	0.01%	0.001%
5	2.767	534	537	541	rBV	334	292	0.02%	0.002%
6	2.819	550	553	556	rVB2	206	106	0.01%	0.001%
7	2.912	579	582	584	rVB2	224	128	0.01%	0.001%
8	2.925	584	586	588	rBV	177	92	0.00%	0.001%
9	2.999	606	609	613	rVB	305	189	0.01%	0.001%
10	3.018	613	615	616	rBV	196	84	0.00%	0.001%
11	3.118	644	646	648	rVB	388	143	0.01%	0.001%
12	3.269	691	693	696	rVB	121	55	0.00%	0.000%
13	3.288	696	699	701	rBV	197	129	0.01%	0.001%
14	3.320	705	709	714	rBV2	257	329	0.02%	0.002%
15	3.372	722	725	726	rBV2	135	63	0.00%	0.000%
16	3.404	733	735	736	rBV2	178	61	0.00%	0.000%
17	3.458	749	752	756	rBV2	158	161	0.01%	0.001%
18	3.487	759	761	764	rVB2	208	100	0.01%	0.001%
19	3.513	764	769	772	rBV2	161	140	0.01%	0.001%
20	3.597	790	795	798	rBV3	265	192	0.01%	0.001%
21	3.645	807	810	812	rBV2	187	108	0.01%	0.001%
22	3.706	827	829	831	rVB	72	31	0.00%	0.000%
23	3.741	834	840	843	rBV3	297	310	0.02%	0.002%
24	3.786	846	854	888	rBV	125909	359636	19.06%	2.638%
25	4.249	982	998	1026	rBV	297439	766038	40.59%	5.618%
26	4.690	1133	1135	1137	rBV2	366	129	0.01%	0.001%
27	4.883	1193	1195	1201	rBV3	404	450	0.02%	0.003%
28	4.957	1201	1218	1259	rBV2	710675	1887291	100.00%	13.842%
29	5.394	1352	1354	1356	rBV3	373	170	0.01%	0.001%
30	5.445	1367	1370	1373	rBV2	275	224	0.01%	0.002%
31	5.532	1386	1397	1440	rBV	444097	938382	49.72%	6.882%
32	5.835	1481	1491	1511	rBV4	9427	22514	1.19%	0.165%
33	5.937	1521	1523	1525	rBV2	320	170	0.01%	0.001%
34	5.986	1526	1538	1579	rVV	407592	861555	45.65%	6.319%
35	6.397	1663	1666	1668	rBV3	456	278	0.01%	0.002%
36	6.413	1669	1671	1675	rVV2	405	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035377.D
 Acq On : 24 Apr 2024 11:19
 Operator : SY/MD
 Sample : P2234-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.439	1678	1679	1680	rBV2	244	74	0.00%	0.001%
38	6.487	1690	1694	1696	rVB	301	203	0.01%	0.001%
39	6.507	1696	1700	1701	rBV	190	102	0.01%	0.001%
40	6.539	1706	1710	1711	rBV	142	94	0.00%	0.001%
41	6.574	1717	1721	1722	rBV2	435	222	0.01%	0.002%
42	6.616	1730	1734	1736	rVB	296	179	0.01%	0.001%
43	6.642	1738	1742	1747	rBV3	530	463	0.02%	0.003%
44	6.687	1754	1756	1759	rVB2	432	198	0.01%	0.001%
45	6.722	1759	1767	1770	rBV3	545	655	0.03%	0.005%
46	6.744	1770	1774	1775	rBV2	388	225	0.01%	0.002%
47	6.777	1782	1784	1785	rBV2	198	103	0.01%	0.001%
48	6.796	1788	1790	1793	rVB2	210	99	0.01%	0.001%
49	6.822	1793	1798	1801	rBV	296	286	0.02%	0.002%
50	6.876	1811	1815	1816	rBV2	253	156	0.01%	0.001%
51	6.912	1816	1826	1868	rVV	201749	393499	20.85%	2.886%
52	7.137	1894	1896	1898	rBV3	301	114	0.01%	0.001%
53	7.243	1917	1929	1968	rBV	812704	1451176	76.89%	10.643%
54	7.551	2016	2025	2055	rBV	140122	265119	14.05%	1.944%
55	7.915	2134	2138	2140	rBV	501	351	0.02%	0.003%
56	7.979	2156	2158	2162	rVB2	399	241	0.01%	0.002%
57	8.024	2163	2172	2223	rBV2	336797	812521	43.05%	5.959%
58	8.513	2321	2324	2325	rBV2	524	304	0.02%	0.002%
59	8.561	2336	2339	2342	rBV4	460	363	0.02%	0.003%
60	8.629	2357	2360	2362	rBV2	520	335	0.02%	0.002%
61	8.719	2386	2388	2391	rBV2	251	171	0.01%	0.001%
62	8.735	2391	2393	2394	rBV2	289	126	0.01%	0.001%
63	8.783	2397	2408	2442	rBV	709122	1184318	62.75%	8.686%
64	9.175	2527	2530	2532	rBV3	227	154	0.01%	0.001%
65	9.188	2532	2534	2537	rVV2	271	148	0.01%	0.001%
66	9.223	2543	2545	2552	rVB2	575	440	0.02%	0.003%
67	9.288	2563	2565	2572	rVB3	482	473	0.03%	0.003%
68	9.317	2572	2574	2575	rBV3	289	131	0.01%	0.001%
69	9.336	2578	2580	2581	rBV	139	39	0.00%	0.000%
70	9.378	2589	2593	2598	rBV2	352	336	0.02%	0.002%
71	9.490	2624	2628	2629	rBV	448	319	0.02%	0.002%
72	9.719	2696	2699	2706	rVB3	282	275	0.01%	0.002%
73	9.805	2723	2726	2729	rBV2	205	157	0.01%	0.001%
74	9.973	2775	2778	2780	rBV	219	115	0.01%	0.001%
75	10.021	2789	2793	2795	rBV	219	189	0.01%	0.001%
76	10.101	2815	2818	2820	rBV2	223	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035377.D
 Acq On : 24 Apr 2024 11:19
 Operator : SY/MD
 Sample : P2234-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2820	2833	2861	rVV	604417	956367	50.67%	7.014%
78	10.413	2913	2915	2917	rVB2	176	50	0.00%	0.000%
79	10.426	2917	2919	2921	rBV	130	64	0.00%	0.000%
80	10.448	2923	2926	2931	rVB3	354	287	0.02%	0.002%
81	10.484	2934	2937	2938	rBV	606	337	0.02%	0.002%
82	10.526	2949	2950	2952	rBV	213	109	0.01%	0.001%
83	10.584	2967	2968	2969	rBV	205	50	0.00%	0.000%
84	10.783	3027	3030	3032	rBV2	546	318	0.02%	0.002%
85	11.072	3117	3120	3123	rBV	421	259	0.01%	0.002%
86	11.127	3134	3137	3143	rVB4	1723	1705	0.09%	0.013%
87	11.182	3144	3154	3181	rBV	687438	1103880	58.49%	8.096%
88	11.558	3259	3271	3296	rBV	871811	1376854	72.95%	10.098%
89	11.796	3341	3345	3348	rBV4	750	525	0.03%	0.004%
90	11.870	3365	3368	3369	rBV	563	339	0.02%	0.002%
91	11.940	3387	3390	3392	rVB2	332	197	0.01%	0.001%
92	12.278	3492	3495	3496	rBV2	357	169	0.01%	0.001%
93	12.503	3558	3565	3566	rBV2	351	452	0.02%	0.003%
94	12.693	3621	3624	3628	rBV2	423	369	0.02%	0.003%
95	13.146	3763	3765	3770	rVB2	387	214	0.01%	0.002%
96	13.204	3776	3783	3798	rVB4	8108	13389	0.71%	0.098%
97	13.445	3850	3858	3879	rVB	16554	28853	1.53%	0.212%
98	13.683	3924	3932	3941	rBV4	6230	10228	0.54%	0.075%
99	13.754	3949	3954	3957	rBV3	699	631	0.03%	0.005%
100	13.841	3978	3981	3985	rBV3	587	416	0.02%	0.003%




Sum of corrected areas: 13634548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035377.D
Acq On : 24 Apr 2024 11:19
Operator : SY/MD
Sample : P2234-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

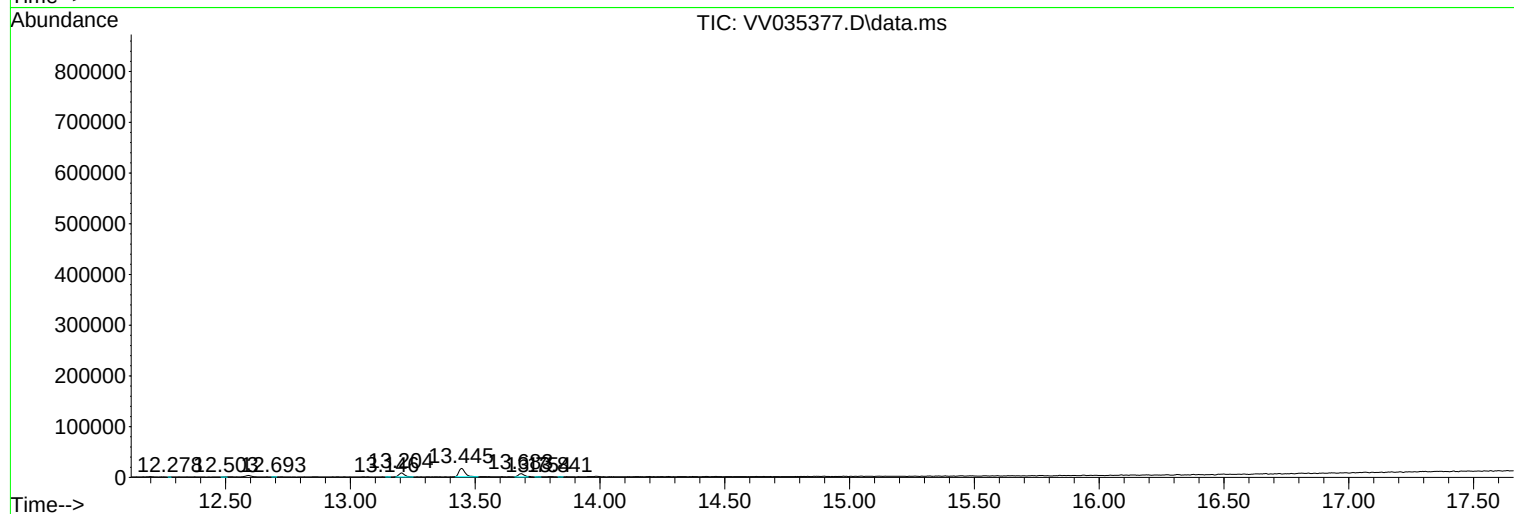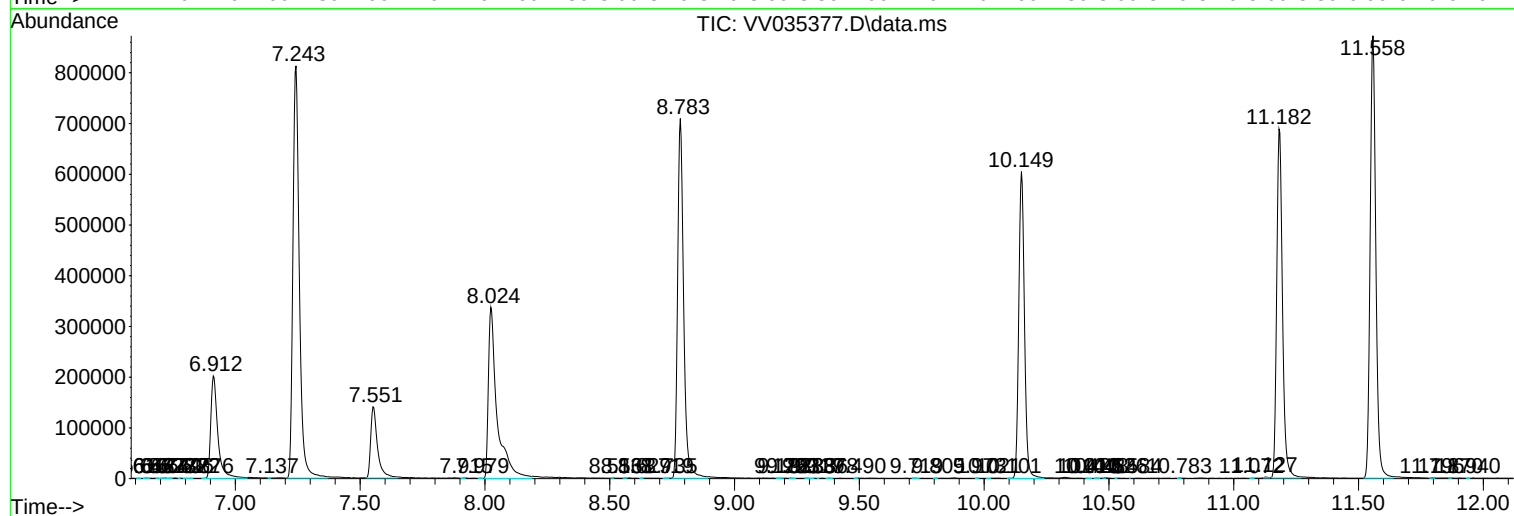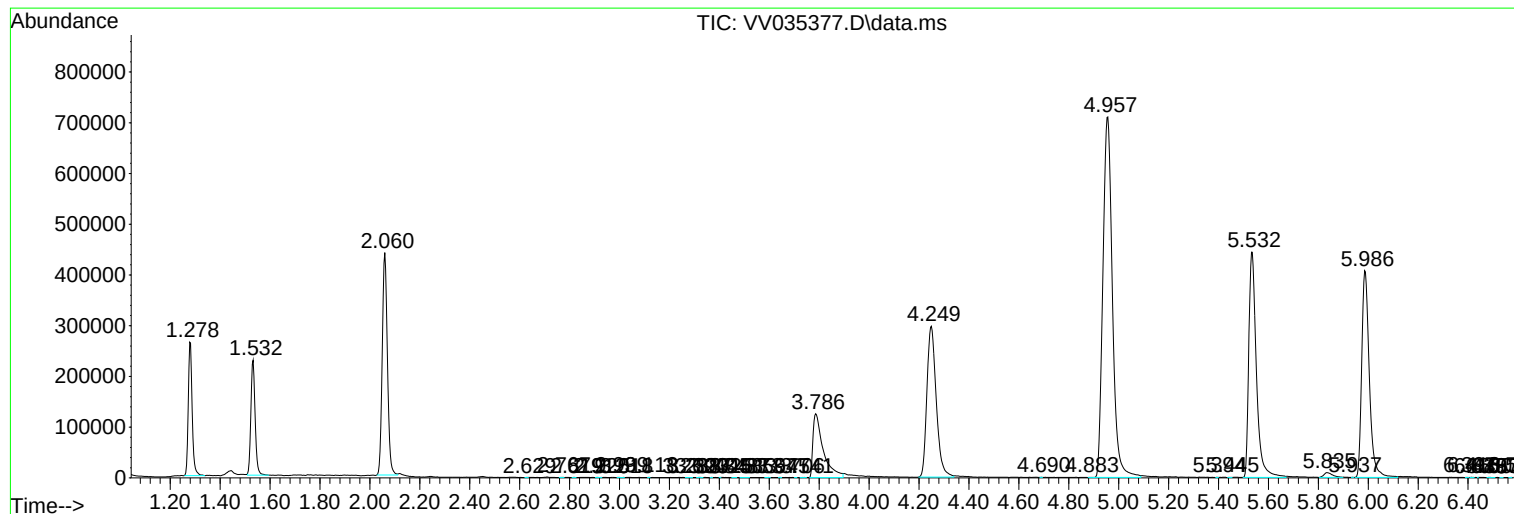

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035377.D
Acq On : 24 Apr 2024 11:19
Operator : SY/MD
Sample : P2234-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035377.D
Acq On : 24 Apr 2024 11:19
Operator : SY/MD
Sample : P2234-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------