

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035378.D
 Acq On : 24 Apr 2024 11:42
 Operator : SY/MD
 Sample : P2234-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rVB	251141	264976	14.59%	2.033%
2	1.532	146	153	170	rVB	216703	259896	14.31%	1.994%
3	2.059	308	317	336	rBV	414402	591556	32.57%	4.538%
4	2.452	430	439	448	rBV2	4073	6270	0.35%	0.048%
5	2.510	453	457	460	rBV	350	288	0.02%	0.002%
6	2.703	515	517	522	rVB5	922	661	0.04%	0.005%
7	2.741	526	529	530	rBV	166	76	0.00%	0.001%
8	2.940	589	591	593	rBV	233	98	0.01%	0.001%
9	2.979	600	603	604	rBV2	266	152	0.01%	0.001%
10	3.069	628	631	635	rVB2	286	246	0.01%	0.002%
11	3.092	635	638	641	rBV3	192	128	0.01%	0.001%
12	3.108	641	643	645	rBV	312	151	0.01%	0.001%
13	3.140	651	653	654	rBV	115	30	0.00%	0.000%
14	3.246	681	686	689	rBV2	135	140	0.01%	0.001%
15	3.272	689	694	698	rBV2	342	349	0.02%	0.003%
16	3.336	711	714	716	rBV2	191	112	0.01%	0.001%
17	3.407	732	736	739	rBV2	143	116	0.01%	0.001%
18	3.423	739	741	745	rVB	274	181	0.01%	0.001%
19	3.484	758	760	761	rBV	152	66	0.00%	0.001%
20	3.535	773	776	778	rBV	195	126	0.01%	0.001%
21	3.580	788	790	793	rVB	150	67	0.00%	0.001%
22	3.622	800	803	807	rBV2	193	137	0.01%	0.001%
23	3.645	807	810	813	rVB2	183	104	0.01%	0.001%
24	3.664	813	816	818	rBV2	201	128	0.01%	0.001%
25	3.680	819	821	824	rVB2	194	110	0.01%	0.001%
26	3.696	824	826	829	rBV2	151	91	0.01%	0.001%
27	3.735	833	838	840	rBV2	217	189	0.01%	0.001%
28	3.751	841	843	846	rVB2	185	66	0.00%	0.001%
29	3.786	846	854	896	rBV	127430	374778	20.64%	2.875%
30	4.249	983	998	1034	rBV	283947	732622	40.34%	5.621%
31	4.699	1137	1138	1139	rBV	268	76	0.00%	0.001%
32	4.818	1173	1175	1176	rBV	211	82	0.00%	0.001%
33	4.956	1201	1218	1267	rBV2	685494	1816061	100.00%	13.933%
34	5.535	1387	1398	1437	rBV	410439	874455	48.15%	6.709%
35	5.837	1482	1492	1509	rBV6	7890	18992	1.05%	0.146%
36	5.985	1525	1538	1576	rBV	396164	830940	45.76%	6.375%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035378.D
 Acq On : 24 Apr 2024 11:42
 Operator : SY/MD
 Sample : P2234-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.358	1652	1654	1657	rBV2	330	215	0.01%	0.002%
38	6.413	1668	1671	1672	rBV2	223	120	0.01%	0.001%
39	6.442	1677	1680	1681	rBV	157	77	0.00%	0.001%
40	6.448	1681	1682	1684	rVV	344	133	0.01%	0.001%
41	6.461	1684	1686	1689	rVB2	244	104	0.01%	0.001%
42	6.477	1689	1691	1695	rBV2	239	143	0.01%	0.001%
43	6.513	1701	1702	1703	rBV	117	25	0.00%	0.000%
44	6.529	1703	1707	1709	rBV3	311	255	0.01%	0.002%
45	6.567	1716	1719	1723	rBV3	303	294	0.02%	0.002%
46	6.612	1730	1733	1735	rBV	234	149	0.01%	0.001%
47	6.628	1736	1738	1741	rVB	264	112	0.01%	0.001%
48	6.648	1741	1744	1746	rBV	399	253	0.01%	0.002%
49	6.664	1746	1749	1752	rBV3	448	294	0.02%	0.002%
50	6.709	1760	1763	1764	rBV	308	201	0.01%	0.002%
51	6.747	1772	1775	1778	rBV2	375	302	0.02%	0.002%
52	6.786	1785	1787	1789	rBV	216	119	0.01%	0.001%
53	6.828	1795	1800	1803	rBV2	259	226	0.01%	0.002%
54	6.873	1806	1814	1816	rBV2	226	264	0.01%	0.002%
55	6.911	1816	1826	1852	rBV	190271	370654	20.41%	2.844%
56	7.243	1918	1929	1956	rBV	771751	1362665	75.03%	10.454%
57	7.551	2016	2025	2057	rBV	135420	255387	14.06%	1.959%
58	7.796	2099	2101	2103	rBV2	368	112	0.01%	0.001%
59	7.908	2134	2136	2140	rVB2	484	311	0.02%	0.002%
60	7.963	2152	2153	2156	rVB3	311	120	0.01%	0.001%
61	7.979	2156	2158	2160	rBV3	131	56	0.00%	0.000%
62	8.024	2163	2172	2225	rBV2	351907	823968	45.37%	6.322%
63	8.484	2313	2315	2319	rBV3	473	289	0.02%	0.002%
64	8.561	2335	2339	2341	rBV3	883	623	0.03%	0.005%
65	8.783	2397	2408	2441	rBV	662916	1117682	61.54%	8.575%
66	9.349	2578	2584	2585	rBV3	419	315	0.02%	0.002%
67	9.416	2602	2605	2607	rBV2	203	138	0.01%	0.001%
68	9.484	2624	2626	2630	rBV4	414	326	0.02%	0.003%
69	9.577	2652	2655	2661	rBV3	343	350	0.02%	0.003%
70	9.670	2682	2684	2686	rBV	265	125	0.01%	0.001%
71	9.715	2695	2698	2702	rVB2	266	186	0.01%	0.001%
72	9.738	2702	2705	2707	rBV	242	141	0.01%	0.001%
73	9.754	2707	2710	2712	rVV	282	128	0.01%	0.001%
74	9.796	2720	2723	2725	rBV	258	182	0.01%	0.001%
75	10.078	2807	2811	2813	rBV2	264	163	0.01%	0.001%
76	10.091	2813	2815	2818	rBV	262	124	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035378.D
 Acq On : 24 Apr 2024 11:42
 Operator : SY/MD
 Sample : P2234-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2868	rVV	595854	948786	52.24%	7.279%
78	10.541	2953	2955	2957	rBV	189	108	0.01%	0.001%
79	10.567	2960	2963	2970	rBV2	267	290	0.02%	0.002%
80	10.625	2978	2981	2984	rBV	280	203	0.01%	0.002%
81	10.644	2985	2987	2991	rVB	311	157	0.01%	0.001%
82	10.667	2991	2994	2995	rBV	288	172	0.01%	0.001%
83	10.722	3007	3011	3016	rBV2	279	287	0.02%	0.002%
84	10.789	3029	3032	3036	rVB2	420	296	0.02%	0.002%
85	10.998	3091	3097	3101	rBV2	429	383	0.02%	0.003%
86	11.185	3144	3155	3185	rBV	646231	1032121	56.83%	7.919%
87	11.458	3237	3240	3241	rBV	457	231	0.01%	0.002%
88	11.557	3259	3271	3299	rBV	809499	1308533	72.05%	10.039%
89	11.959	3394	3396	3397	rBV	309	108	0.01%	0.001%
90	12.033	3417	3419	3420	rBV	205	84	0.00%	0.001%
91	13.165	3769	3771	3772	rBV	407	150	0.01%	0.001%
92	13.207	3777	3784	3800	rVB3	5706	9448	0.52%	0.072%
93	13.313	3815	3817	3825	rVB3	485	366	0.02%	0.003%
94	13.448	3852	3859	3868	rBV2	7925	13418	0.74%	0.103%
95	13.686	3927	3933	3947	rVB3	4268	7262	0.40%	0.056%




Sum of corrected areas: 13034250

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035378.D
Acq On : 24 Apr 2024 11:42
Operator : SY/MD
Sample : P2234-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

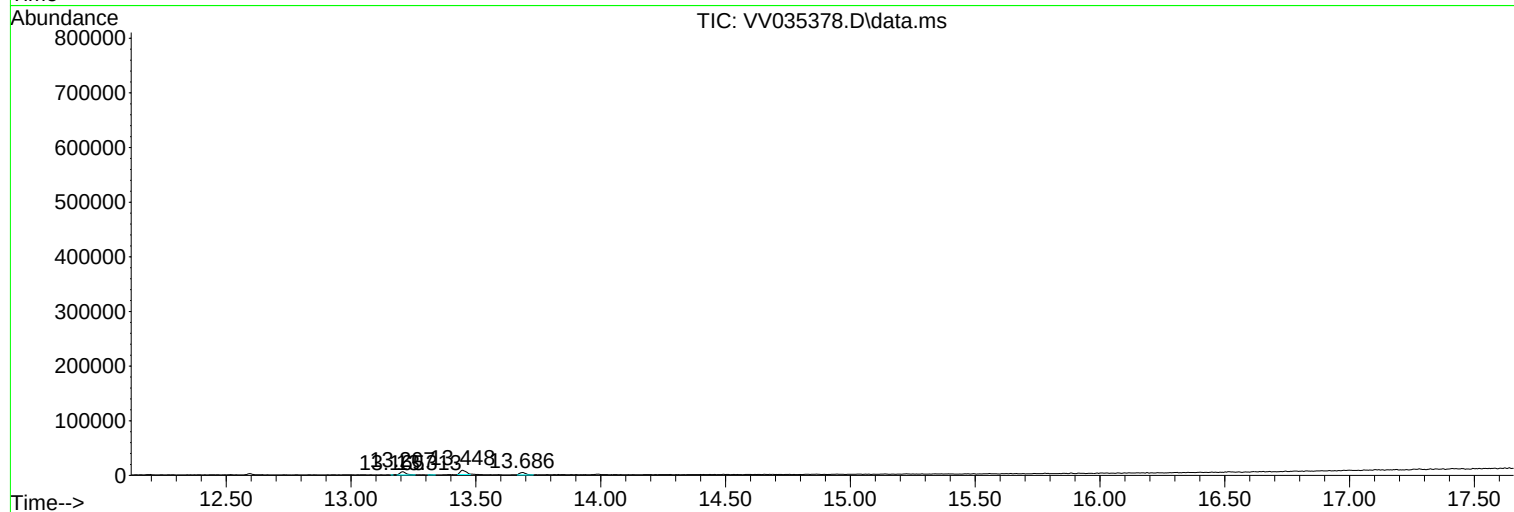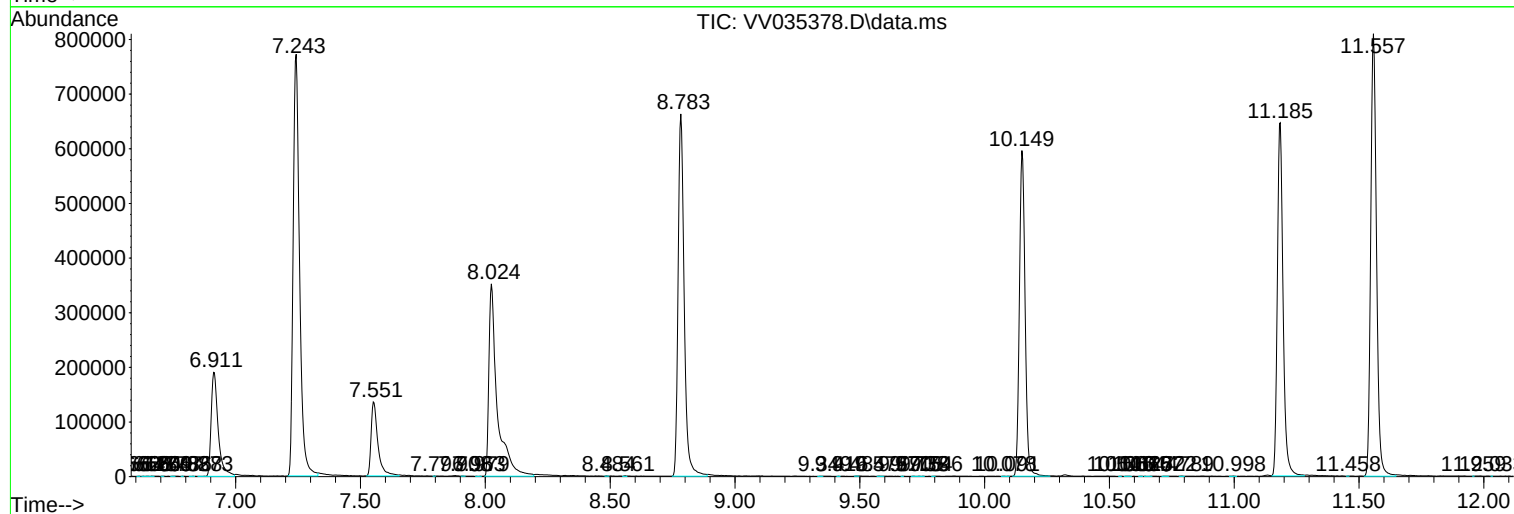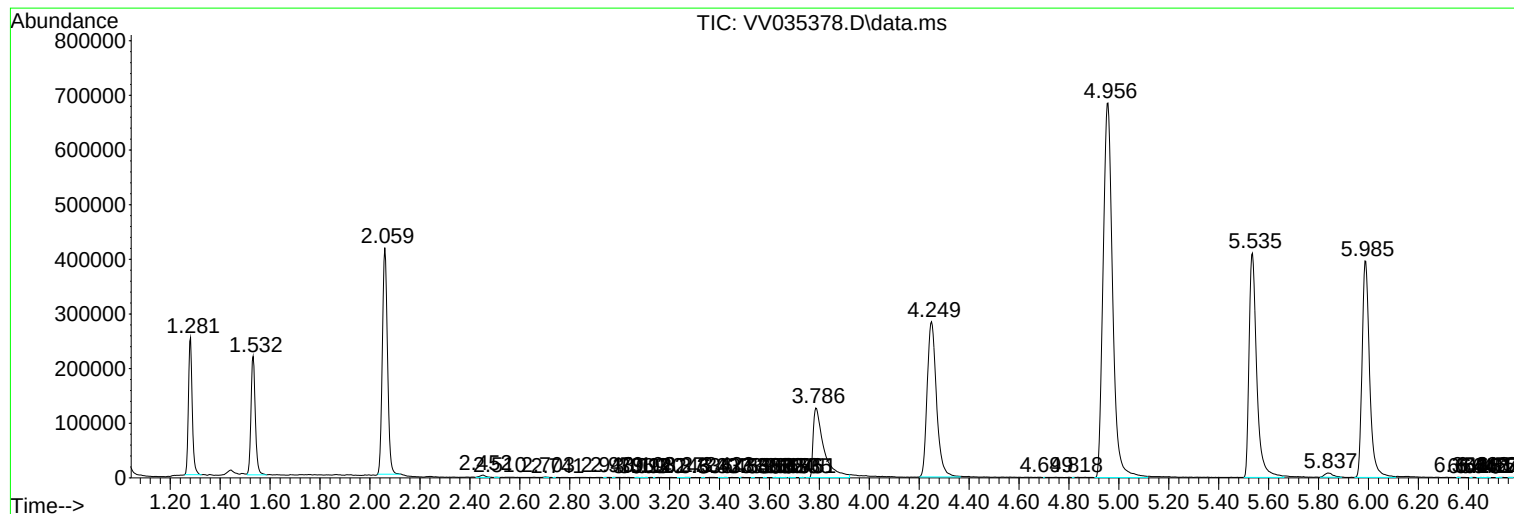

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035378.D
Acq On : 24 Apr 2024 11:42
Operator : SY/MD
Sample : P2234-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035378.D
Acq On : 24 Apr 2024 11:42
Operator : SY/MD
Sample : P2234-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc