

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035379.D
 Acq On : 24 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	53	rBV	28605	26869	1.50%	0.207%
2	1.278	67	74	92	rVB	259444	280091	15.60%	2.153%
3	1.532	145	153	169	rVB	218080	256505	14.29%	1.971%
4	2.059	307	317	330	rBV	412514	602694	33.57%	4.632%
5	2.445	433	437	445	rBV6	1340	1811	0.10%	0.014%
6	2.770	535	538	539	rBV	208	112	0.01%	0.001%
7	2.883	568	573	574	rBV4	411	350	0.02%	0.003%
8	2.940	587	591	593	rBV2	447	319	0.02%	0.002%
9	3.018	612	615	617	rBV	294	185	0.01%	0.001%
10	3.031	617	619	622	rVV2	391	209	0.01%	0.002%
11	3.059	624	628	630	rVB2	348	238	0.01%	0.002%
12	3.082	630	635	639	rBV2	490	437	0.02%	0.003%
13	3.146	652	655	657	rBV	204	125	0.01%	0.001%
14	3.204	672	673	674	rBV	150	32	0.00%	0.000%
15	3.262	688	691	693	rBV	291	196	0.01%	0.002%
16	3.371	723	725	729	rBV2	259	115	0.01%	0.001%
17	3.397	729	733	736	rBV	328	250	0.01%	0.002%
18	3.416	736	739	740	rBV	236	118	0.01%	0.001%
19	3.510	767	768	769	rVB	245	47	0.00%	0.000%
20	3.519	769	771	773	rBV2	94	57	0.00%	0.000%
21	3.535	773	776	778	rBV	134	102	0.01%	0.001%
22	3.686	819	823	831	rBV	259	303	0.02%	0.002%
23	3.725	831	835	837	rBV	207	161	0.01%	0.001%
24	3.786	845	854	893	rBV	122626	358926	19.99%	2.759%
25	4.249	981	998	1030	rBV2	297223	854367	47.58%	6.567%
26	4.735	1142	1149	1153	rBV3	552	695	0.04%	0.005%
27	4.953	1202	1217	1260	rBV2	674665	1795517	100.00%	13.800%
28	5.442	1360	1369	1371	rBV4	532	645	0.04%	0.005%
29	5.532	1386	1397	1445	rBV	401504	857733	47.77%	6.592%
30	5.831	1481	1490	1509	rBV2	8376	20341	1.13%	0.156%
31	5.985	1525	1538	1569	rBV	390380	815667	45.43%	6.269%
32	6.378	1656	1660	1663	rBV2	460	374	0.02%	0.003%
33	6.442	1669	1680	1696	rBV3	12135	25643	1.43%	0.197%
34	6.574	1714	1721	1725	rBV2	423	405	0.02%	0.003%
35	6.593	1725	1727	1730	rVB2	383	200	0.01%	0.002%
36	6.609	1730	1732	1733	rBV	163	44	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035379.D
 Acq On : 24 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.632	1734	1739	1741	rBV3	536	527	0.03%	0.004%
38	6.657	1745	1747	1749	rBV2	306	135	0.01%	0.001%
39	6.876	1812	1815	1816	rBV	171	100	0.01%	0.001%
40	6.911	1816	1826	1857	rBV	192547	371665	20.70%	2.857%
41	7.243	1918	1929	1976	rBV	765095	1375697	76.62%	10.573%
42	7.551	2016	2025	2056	rBV	131913	253551	14.12%	1.949%
43	7.853	2117	2119	2121	rBV2	430	182	0.01%	0.001%
44	7.937	2144	2145	2148	rVB	309	125	0.01%	0.001%
45	7.953	2148	2150	2152	rBV	289	109	0.01%	0.001%
46	7.963	2152	2153	2155	rVB	125	27	0.00%	0.000%
47	7.976	2155	2157	2158	rBV	262	100	0.01%	0.001%
48	7.989	2158	2161	2163	rBV2	331	256	0.01%	0.002%
49	8.024	2163	2172	2214	rBV2	332525	777446	43.30%	5.975%
50	8.542	2327	2333	2335	rBV4	425	323	0.02%	0.002%
51	8.587	2345	2347	2349	rVB	484	156	0.01%	0.001%
52	8.609	2349	2354	2356	rBV3	431	338	0.02%	0.003%
53	8.689	2377	2379	2381	rVB	215	86	0.00%	0.001%
54	8.741	2391	2395	2397	rBV	420	306	0.02%	0.002%
55	8.783	2397	2408	2439	rBV	643988	1082713	60.30%	8.322%
56	9.011	2477	2479	2483	rVB2	463	168	0.01%	0.001%
57	9.053	2490	2492	2495	rBV3	418	221	0.01%	0.002%
58	9.165	2524	2527	2530	rVB2	397	226	0.01%	0.002%
59	9.220	2540	2544	2546	rBV2	321	232	0.01%	0.002%
60	9.252	2553	2554	2556	rVB2	292	87	0.00%	0.001%
61	9.265	2556	2558	2560	rBV2	97	46	0.00%	0.000%
62	9.307	2570	2571	2575	rVB2	281	145	0.01%	0.001%
63	9.333	2575	2579	2584	rVB2	356	348	0.02%	0.003%
64	9.358	2584	2587	2590	rBV3	403	239	0.01%	0.002%
65	9.384	2590	2595	2601	rVB2	375	462	0.03%	0.004%
66	9.410	2601	2603	2604	rBV2	240	79	0.00%	0.001%
67	9.497	2625	2630	2631	rBV2	498	410	0.02%	0.003%
68	9.519	2634	2637	2639	rBV2	696	415	0.02%	0.003%
69	9.599	2658	2662	2667	rVB3	363	325	0.02%	0.002%
70	9.648	2675	2677	2680	rBV	175	105	0.01%	0.001%
71	9.686	2685	2689	2691	rBV2	268	194	0.01%	0.001%
72	9.728	2700	2702	2705	rVB3	268	135	0.01%	0.001%
73	9.776	2714	2717	2719	rBV	209	128	0.01%	0.001%
74	9.857	2740	2742	2744	rBV2	213	126	0.01%	0.001%
75	9.956	2768	2773	2776	rBV3	267	257	0.01%	0.002%
76	10.040	2796	2799	2800	rBV2	230	120	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035379.D
 Acq On : 24 Apr 2024 12:05
 Operator : SY/MD
 Sample : P2235-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.101	2814	2818	2821	rBV2	567	502	0.03%	0.004%
78	10.149	2822	2833	2863	rVV	577561	919571	51.21%	7.068%
79	10.320	2881	2886	2887	rBV2	1842	1344	0.07%	0.010%
80	10.580	2964	2967	2968	rBV2	163	108	0.01%	0.001%
81	10.619	2976	2979	2987	rVB2	337	377	0.02%	0.003%
82	10.664	2987	2993	2995	rBV2	250	257	0.01%	0.002%
83	10.715	3003	3009	3016	rVB3	581	719	0.04%	0.006%
84	10.786	3029	3031	3036	rBV2	322	218	0.01%	0.002%
85	10.902	3066	3067	3068	rBV2	159	48	0.00%	0.000%
86	10.914	3069	3071	3073	rVB	239	93	0.01%	0.001%
87	11.104	3128	3130	3132	rBV2	307	149	0.01%	0.001%
88	11.130	3132	3138	3140	rVV4	1766	1842	0.10%	0.014%
89	11.185	3144	3155	3189	rVV	632431	1005188	55.98%	7.726%
90	11.464	3239	3242	3246	rBV	576	455	0.03%	0.003%
91	11.558	3259	3271	3298	rBV	814992	1296059	72.18%	9.961%
92	11.950	3391	3393	3394	rBV	318	150	0.01%	0.001%
93	12.184	3462	3466	3467	rBV2	708	482	0.03%	0.004%
94	12.348	3514	3517	3518	rBV	419	210	0.01%	0.002%
95	12.390	3527	3530	3534	rVB3	636	391	0.02%	0.003%
96	12.416	3534	3538	3540	rBV	321	261	0.01%	0.002%
97	12.522	3568	3571	3573	rBV2	458	284	0.02%	0.002%
98	12.590	3586	3592	3604	rBV6	1704	2971	0.17%	0.023%
99	13.107	3751	3753	3755	rBV6	360	190	0.01%	0.001%
100	13.448	3852	3859	3871	rBV2	5412	8887	0.49%	0.068%




Sum of corrected areas: 13010949

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035379.D
Acq On : 24 Apr 2024 12:05
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

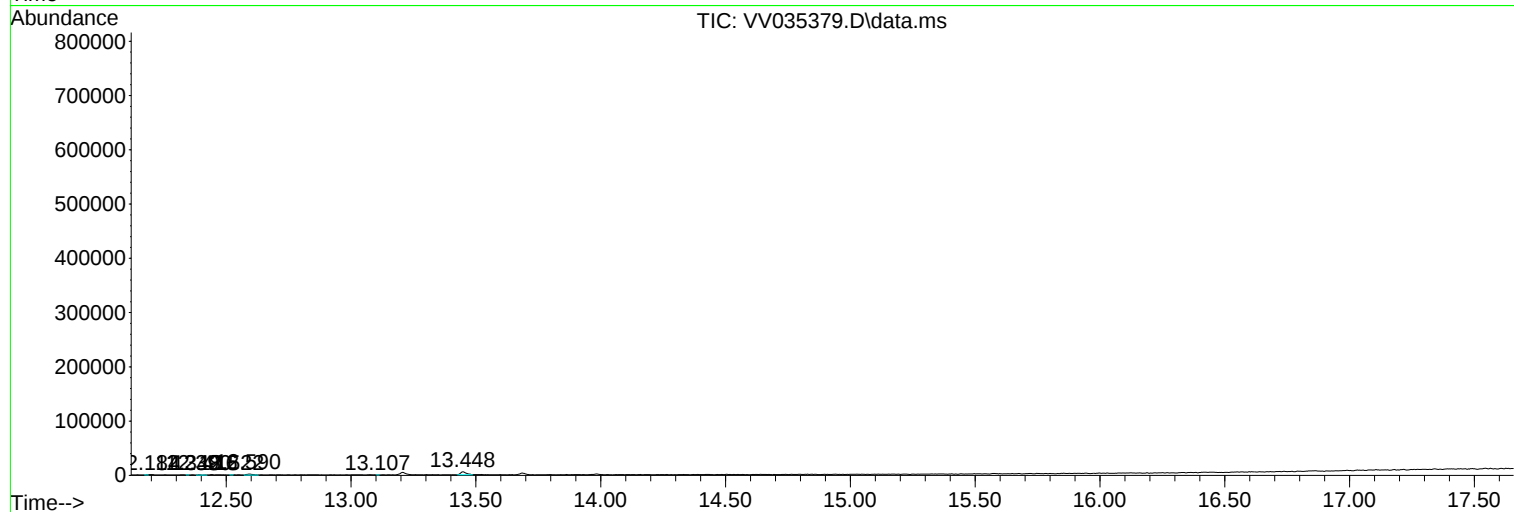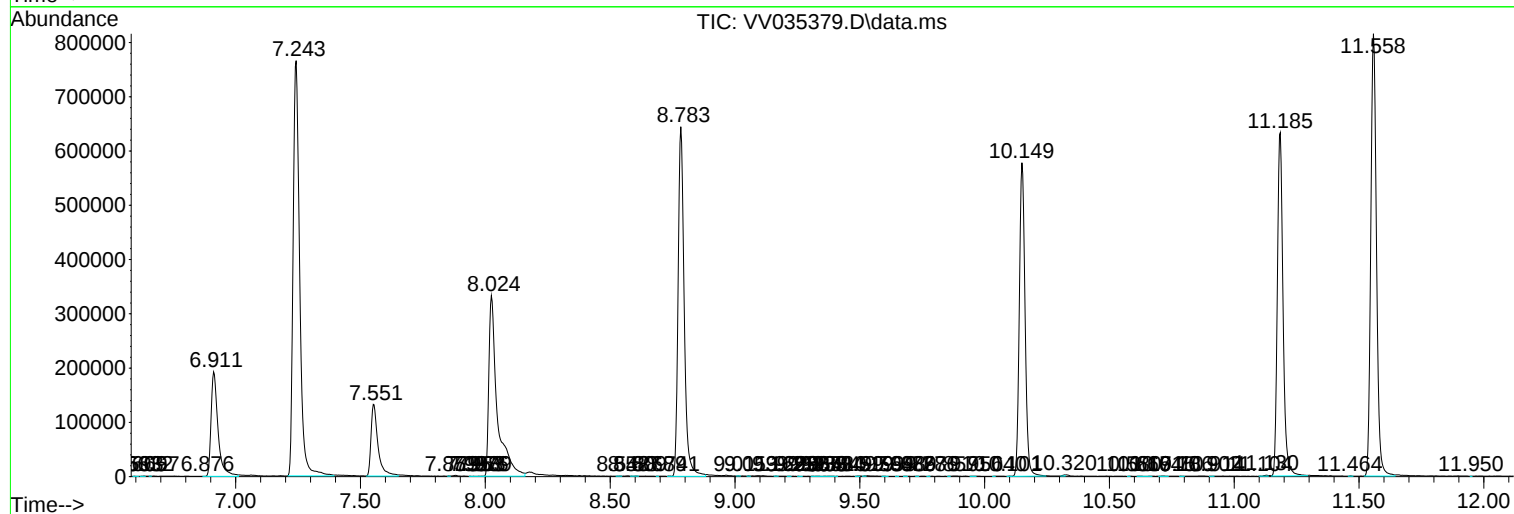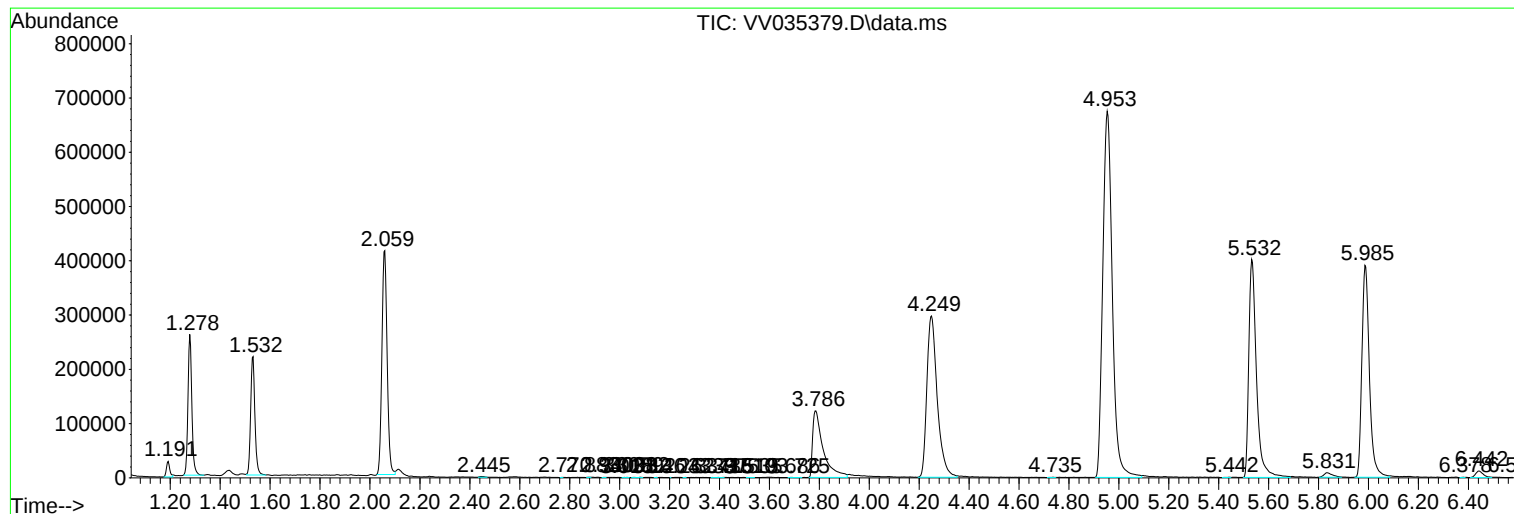

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035379.D
Acq On : 24 Apr 2024 12:05
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035379.D
Acq On : 24 Apr 2024 12:05
Operator : SY/MD
Sample : P2235-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0810

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------