

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035381.D
 Acq On : 24 Apr 2024 12:52
 Operator : SY/MD
 Sample : P2158-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	148100	154852	12.62%	1.798%
2	1.532	147	153	172	rVB	131460	154552	12.59%	1.795%
3	2.059	308	317	334	rVB	238792	347113	28.28%	4.031%
4	2.407	423	425	429	rBV2	438	274	0.02%	0.003%
5	2.706	514	518	519	rBV	369	228	0.02%	0.003%
6	2.831	554	557	563	rVB3	302	308	0.03%	0.004%
7	2.867	564	568	570	rBV2	394	295	0.02%	0.003%
8	2.966	597	599	600	rBV	285	155	0.01%	0.002%
9	3.021	613	616	621	rBV2	276	293	0.02%	0.003%
10	3.076	630	633	635	rBV2	214	122	0.01%	0.001%
11	3.095	635	639	642	rVV	268	231	0.02%	0.003%
12	3.121	642	647	651	rVV	554	505	0.04%	0.006%
13	3.153	653	657	659	rVV2	357	247	0.02%	0.003%
14	3.172	661	663	668	rVB3	168	118	0.01%	0.001%
15	3.198	668	671	677	rBV	167	162	0.01%	0.002%
16	3.230	678	681	687	rBV2	204	175	0.01%	0.002%
17	3.301	698	703	706	rBV2	444	340	0.03%	0.004%
18	3.384	726	729	734	rBV2	199	156	0.01%	0.002%
19	3.445	744	748	754	rBV2	348	329	0.03%	0.004%
20	3.487	760	761	770	rVB2	224	197	0.02%	0.002%
21	3.529	770	774	778	rBV2	317	370	0.03%	0.004%
22	3.635	805	807	811	rVB	305	142	0.01%	0.002%
23	3.661	812	815	822	rVB3	481	447	0.04%	0.005%
24	3.709	824	830	834	rVB3	314	323	0.03%	0.004%
25	3.802	850	859	898	rBV2	63254	214294	17.46%	2.489%
26	4.249	984	998	1027	rBV	160088	414078	33.74%	4.809%
27	4.503	1073	1077	1078	rBV2	426	310	0.03%	0.004%
28	4.561	1092	1095	1098	rBV2	497	363	0.03%	0.004%
29	4.741	1144	1151	1159	rVB4	714	1102	0.09%	0.013%
30	4.825	1175	1177	1181	rBV3	302	213	0.02%	0.002%
31	4.905	1199	1202	1203	rBV2	390	207	0.02%	0.002%
32	4.957	1203	1218	1227	rBV2	393843	981157	79.94%	11.395%
33	5.468	1373	1377	1380	rBV2	528	455	0.04%	0.005%
34	5.535	1388	1398	1430	rBV	264634	561499	45.75%	6.521%
35	5.834	1484	1491	1493	rBV3	3162	3482	0.28%	0.040%
36	5.989	1526	1539	1580	rBV	221309	472321	38.48%	5.485%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042424\
 Data File : VW035381.D
 Acq On : 24 Apr 2024 12:52
 Operator : SY/MD
 Sample : P2158-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.214	1607	1609	1611	rBV2	449	269	0.02%	0.003%
38	6.297	1632	1635	1636	rBV2	227	123	0.01%	0.001%
39	6.416	1670	1672	1675	rBV3	190	115	0.01%	0.001%
40	6.481	1687	1692	1694	rBV2	323	359	0.03%	0.004%
41	6.516	1699	1703	1707	rVB	239	223	0.02%	0.003%
42	6.664	1747	1749	1752	rBV2	182	105	0.01%	0.001%
43	6.731	1768	1770	1774	rBV	166	110	0.01%	0.001%
44	6.825	1796	1799	1806	rVB	440	317	0.03%	0.004%
45	6.857	1807	1809	1811	rBV	265	122	0.01%	0.001%
46	6.915	1815	1827	1855	rBV	99484	202566	16.50%	2.353%
47	7.165	1904	1905	1908	rBV2	225	118	0.01%	0.001%
48	7.243	1917	1929	1955	rBV	417695	745875	60.77%	8.662%
49	7.558	2018	2027	2055	rBV	67561	134281	10.94%	1.560%
50	7.902	2132	2134	2138	rVB2	379	172	0.01%	0.002%
51	7.982	2158	2159	2162	rVB2	323	153	0.01%	0.002%
52	8.030	2162	2174	2214	rBV2	166280	432889	35.27%	5.028%
53	8.522	2324	2327	2328	rBV	326	175	0.01%	0.002%
54	8.661	2368	2370	2373	rBV3	319	212	0.02%	0.002%
55	8.741	2392	2395	2398	rBV2	242	195	0.02%	0.002%
56	8.786	2398	2409	2411	rBV	480700	627970	51.16%	7.293%
57	9.226	2541	2546	2548	rVB	539	435	0.04%	0.005%
58	9.239	2548	2550	2551	rBV	323	133	0.01%	0.002%
59	9.291	2563	2566	2568	rBV	307	206	0.02%	0.002%
60	9.313	2571	2573	2575	rBV	254	125	0.01%	0.001%
61	9.378	2589	2593	2595	rBV2	374	310	0.03%	0.004%
62	9.400	2598	2600	2604	rBV	195	163	0.01%	0.002%
63	9.461	2618	2619	2623	rVB2	358	142	0.01%	0.002%
64	9.484	2623	2626	2628	rBV2	254	154	0.01%	0.002%
65	9.522	2634	2638	2639	rBV2	348	218	0.02%	0.003%
66	9.542	2641	2644	2646	rBV	412	208	0.02%	0.002%
67	9.625	2665	2670	2673	rBV3	316	252	0.02%	0.003%
68	9.670	2681	2684	2685	rBV	288	163	0.01%	0.002%
69	9.808	2725	2727	2729	rVB2	243	100	0.01%	0.001%
70	9.931	2763	2765	2769	rBV	261	189	0.02%	0.002%
71	9.966	2773	2776	2781	rVB2	418	365	0.03%	0.004%
72	10.149	2821	2833	2857	rBV	331478	539077	43.92%	6.261%
73	10.410	2912	2914	2917	rBV	276	162	0.01%	0.002%
74	10.471	2929	2933	2937	rBV2	303	336	0.03%	0.004%
75	10.529	2948	2951	2954	rVB	332	183	0.01%	0.002%
76	10.567	2960	2963	2965	rBV2	242	152	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035381.D
 Acq On : 24 Apr 2024 12:52
 Operator : SY/MD
 Sample : P2158-05DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MC0RD2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.670	2993	2995	3000	rVB2	318	247	0.02%	0.003%
78	10.728	3011	3013	3018	rBV2	186	111	0.01%	0.001%
79	10.779	3028	3029	3033	rBV	173	99	0.01%	0.001%
80	10.950	3078	3082	3083	rBV2	207	154	0.01%	0.002%
81	11.040	3106	3110	3115	rBV2	290	316	0.03%	0.004%
82	11.120	3127	3135	3145	rBV2	36975	60317	4.91%	0.701%
83	11.185	3145	3155	3189	rVB2	457495	1075173	87.60%	12.487%
84	11.496	3250	3252	3253	rBV	338	138	0.01%	0.002%
85	11.561	3261	3272	3302	rVB2	558944	1227393	100.00%	14.255%
86	11.815	3349	3351	3355	rVB2	650	447	0.04%	0.005%
87	11.837	3355	3358	3360	rBV2	533	353	0.03%	0.004%
88	11.879	3368	3371	3373	rBV2	488	314	0.03%	0.004%
89	12.075	3427	3432	3436	rBV3	404	373	0.03%	0.004%
90	12.320	3506	3508	3510	rBV	212	124	0.01%	0.001%
91	12.345	3512	3516	3517	rBV	650	451	0.04%	0.005%
92	12.496	3560	3563	3568	rBV4	395	413	0.03%	0.005%
93	12.596	3587	3594	3602	rVB6	1584	2307	0.19%	0.027%
94	12.657	3608	3613	3614	rBV3	363	299	0.02%	0.003%
95	12.686	3618	3622	3623	rBV	759	442	0.04%	0.005%
96	13.120	3755	3757	3762	rBV2	486	412	0.03%	0.005%
97	13.197	3771	3781	3806	rBV	111985	183293	14.93%	2.129%
98	13.393	3839	3842	3845	rBV2	385	271	0.02%	0.003%
99	13.455	3855	3861	3869	rBV3	3114	4268	0.35%	0.050%
100	13.680	3922	3931	3945	rBV3	31526	51845	4.22%	0.602%




Sum of corrected areas: 8610397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035381.D
Acq On : 24 Apr 2024 12:52
Operator : SY/MD
Sample : P2158-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

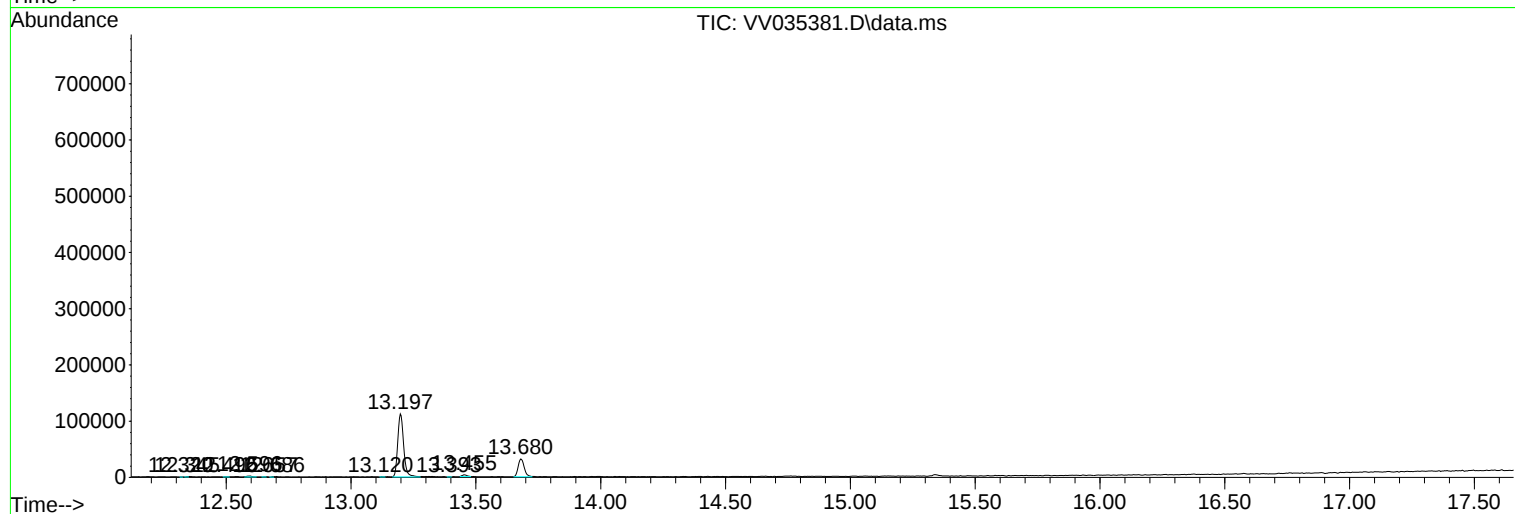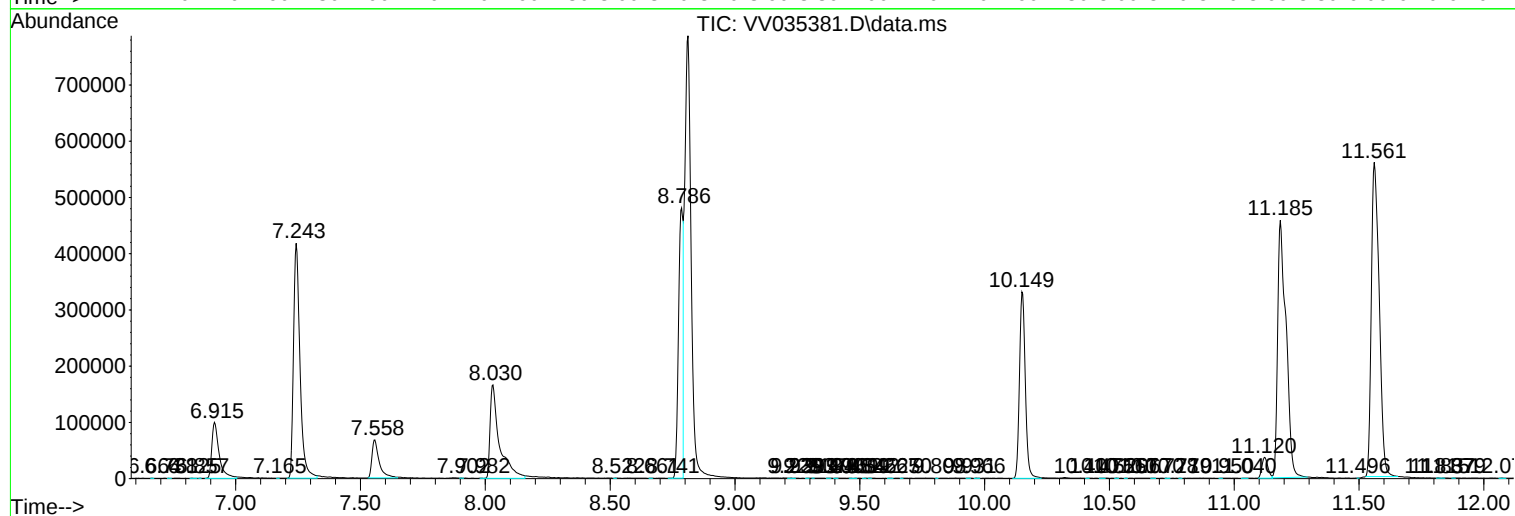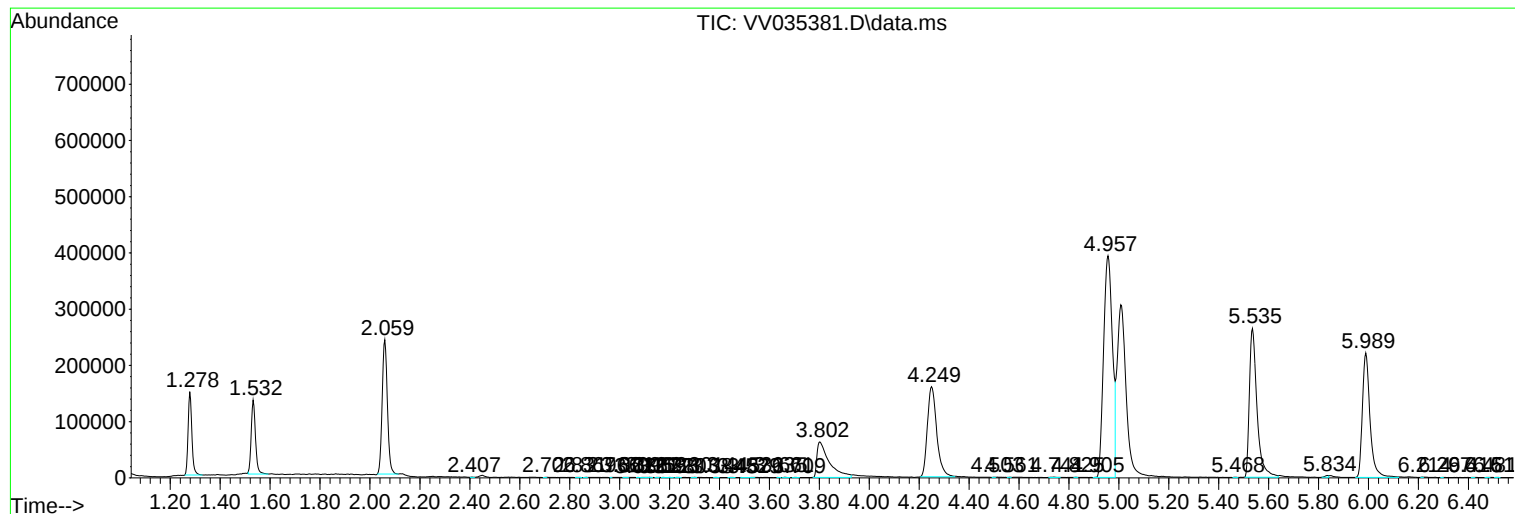

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035381.D
Acq On : 24 Apr 2024 12:52
Operator : SY/MD
Sample : P2158-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035381.D
Acq On : 24 Apr 2024 12:52
Operator : SY/MD
Sample : P2158-05DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RD2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------