

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035383.D
 Acq On : 24 Apr 2024 13:38
 Operator : SY/MD
 Sample : P2235-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	58	rBV	25475	26464	1.47%	0.204%
2	1.278	67	74	89	rVB	252022	271969	15.14%	2.101%
3	1.532	146	153	168	rBV	223670	258798	14.40%	2.000%
4	2.059	307	317	332	rBV	415192	602798	33.55%	4.657%
5	2.558	470	472	473	rBV	337	129	0.01%	0.001%
6	2.706	516	518	522	rVB4	914	618	0.03%	0.005%
7	2.796	544	546	550	rVB2	293	152	0.01%	0.001%
8	2.818	550	553	555	rBV	393	263	0.01%	0.002%
9	2.847	560	562	565	rBV2	259	133	0.01%	0.001%
10	2.867	566	568	571	rVB2	269	160	0.01%	0.001%
11	2.899	571	578	581	rBV5	784	1033	0.06%	0.008%
12	2.950	592	594	598	rBV	238	162	0.01%	0.001%
13	2.979	598	603	604	rBV	322	203	0.01%	0.002%
14	3.031	617	619	623	rVB2	453	246	0.01%	0.002%
15	3.056	623	627	631	rBV	307	258	0.01%	0.002%
16	3.130	646	650	656	rBV2	308	318	0.02%	0.002%
17	3.166	659	661	666	rBV2	237	153	0.01%	0.001%
18	3.240	681	684	687	rBV2	178	145	0.01%	0.001%
19	3.378	724	727	729	rBV2	253	142	0.01%	0.001%
20	3.436	741	745	747	rBV2	266	223	0.01%	0.002%
21	3.449	747	749	754	rVV2	292	219	0.01%	0.002%
22	3.474	754	757	760	rVB3	235	154	0.01%	0.001%
23	3.516	767	770	772	rBV	141	93	0.01%	0.001%
24	3.558	780	783	788	rBV2	274	224	0.01%	0.002%
25	3.590	788	793	795	rBV2	436	327	0.02%	0.003%
26	3.667	814	817	820	rVB2	261	157	0.01%	0.001%
27	3.703	823	828	831	rBV2	154	121	0.01%	0.001%
28	3.754	841	844	845	rBV	142	94	0.01%	0.001%
29	3.796	848	857	903	rBV	112739	372346	20.72%	2.877%
30	4.249	982	998	1036	rBV2	299186	853869	47.53%	6.597%
31	4.709	1139	1141	1145	rVV2	394	173	0.01%	0.001%
32	4.738	1149	1150	1154	rVB2	410	189	0.01%	0.001%
33	4.953	1201	1217	1256	rBV2	677818	1796608	100.00%	13.881%
34	5.259	1310	1312	1313	rBV	410	111	0.01%	0.001%
35	5.336	1333	1336	1337	rBV3	454	306	0.02%	0.002%
36	5.461	1370	1375	1377	rBV2	400	369	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035383.D
 Acq On : 24 Apr 2024 13:38
 Operator : SY/MD
 Sample : P2235-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1440	rBV	380464	823097	45.81%	6.359%
38	5.837	1482	1492	1517	rVB4	8301	21076	1.17%	0.163%
39	5.985	1525	1538	1569	rBV	390992	819811	45.63%	6.334%
40	6.358	1652	1654	1656	rVB2	317	130	0.01%	0.001%
41	6.374	1656	1659	1661	rBV	263	145	0.01%	0.001%
42	6.400	1664	1667	1669	rBV	288	179	0.01%	0.001%
43	6.442	1671	1680	1698	rVB2	11462	23768	1.32%	0.184%
44	6.542	1707	1711	1712	rBV	226	120	0.01%	0.001%
45	6.571	1717	1720	1723	rVB2	199	116	0.01%	0.001%
46	6.706	1757	1762	1766	rVB2	466	365	0.02%	0.003%
47	6.735	1766	1771	1774	rBV3	318	266	0.01%	0.002%
48	6.754	1774	1777	1781	rBV2	277	177	0.01%	0.001%
49	6.818	1794	1797	1799	rBV	240	137	0.01%	0.001%
50	6.911	1815	1826	1859	rBV	189198	368198	20.49%	2.845%
51	7.243	1918	1929	1958	rBV	773910	1366925	76.08%	10.561%
52	7.554	2016	2026	2059	rBV	131633	254088	14.14%	1.963%
53	7.757	2086	2089	2092	rBV3	637	395	0.02%	0.003%
54	7.860	2119	2121	2123	rBV2	645	242	0.01%	0.002%
55	7.918	2136	2139	2142	rVB2	391	236	0.01%	0.002%
56	7.947	2146	2148	2150	rBV	345	162	0.01%	0.001%
57	8.027	2163	2173	2215	rBV2	323761	802707	44.68%	6.202%
58	8.381	2280	2283	2285	rBV4	628	455	0.03%	0.004%
59	8.542	2330	2333	2336	rBV3	753	490	0.03%	0.004%
60	8.783	2397	2408	2449	rBV	624032	1044246	58.12%	8.068%
61	9.091	2500	2504	2506	rBV2	626	520	0.03%	0.004%
62	9.242	2549	2551	2554	rBV2	285	140	0.01%	0.001%
63	9.294	2565	2567	2568	rBV2	216	94	0.01%	0.001%
64	9.374	2590	2592	2594	rBV2	125	84	0.00%	0.001%
65	9.416	2602	2605	2608	rVB	228	136	0.01%	0.001%
66	9.442	2611	2613	2616	rVB2	247	132	0.01%	0.001%
67	9.468	2617	2621	2624	rBV2	154	133	0.01%	0.001%
68	9.484	2624	2626	2628	rBV	274	165	0.01%	0.001%
69	9.496	2628	2630	2637	rVB3	575	464	0.03%	0.004%
70	9.525	2637	2639	2641	rBV2	569	338	0.02%	0.003%
71	9.538	2641	2643	2650	rVB5	504	363	0.02%	0.003%
72	9.606	2661	2664	2669	rVB2	203	126	0.01%	0.001%
73	9.648	2674	2677	2680	rVB	295	181	0.01%	0.001%
74	9.709	2692	2696	2699	rBV	204	166	0.01%	0.001%
75	9.747	2706	2708	2714	rBV2	231	185	0.01%	0.001%
76	9.869	2744	2746	2748	rBV2	235	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035383.D
 Acq On : 24 Apr 2024 13:38
 Operator : SY/MD
 Sample : P2235-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.943	2766	2769	2771	rBV	182	122	0.01%	0.001%
78	10.043	2797	2800	2802	rBV2	198	107	0.01%	0.001%
79	10.149	2822	2833	2862	rBV	588489	930885	51.81%	7.192%
80	10.406	2911	2913	2917	rVB2	300	172	0.01%	0.001%
81	10.423	2917	2918	2921	rBV	181	85	0.00%	0.001%
82	10.484	2932	2937	2939	rBV2	570	595	0.03%	0.005%
83	10.564	2959	2962	2965	rBV3	274	182	0.01%	0.001%
84	10.677	2994	2997	3000	rBV2	274	180	0.01%	0.001%
85	10.715	3003	3009	3010	rBV2	446	426	0.02%	0.003%
86	10.789	3030	3032	3036	rBV2	354	217	0.01%	0.002%
87	10.831	3042	3045	3047	rVB2	188	83	0.00%	0.001%
88	10.850	3048	3051	3053	rBV	287	198	0.01%	0.002%
89	11.095	3125	3127	3130	rBV	157	99	0.01%	0.001%
90	11.120	3131	3135	3136	rBV2	913	621	0.03%	0.005%
91	11.185	3144	3155	3185	rBV	602500	976447	54.35%	7.544%
92	11.512	3255	3257	3259	rBV2	409	275	0.02%	0.002%
93	11.558	3259	3271	3295	rVV	839909	1301422	72.44%	10.055%
94	11.972	3398	3400	3407	rVB3	459	373	0.02%	0.003%
95	12.062	3425	3428	3432	rBV2	290	168	0.01%	0.001%
96	12.191	3465	3468	3469	rBV2	510	291	0.02%	0.002%
97	12.567	3582	3585	3587	rBV3	387	262	0.01%	0.002%
98	12.660	3611	3614	3617	rBV3	334	284	0.02%	0.002%
99	12.805	3657	3659	3663	rVB2	436	202	0.01%	0.002%
100	13.207	3777	3784	3800	rVB5	4925	8518	0.47%	0.066%




Sum of corrected areas: 12942839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035383.D
Acq On : 24 Apr 2024 13:38
Operator : SY/MD
Sample : P2235-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

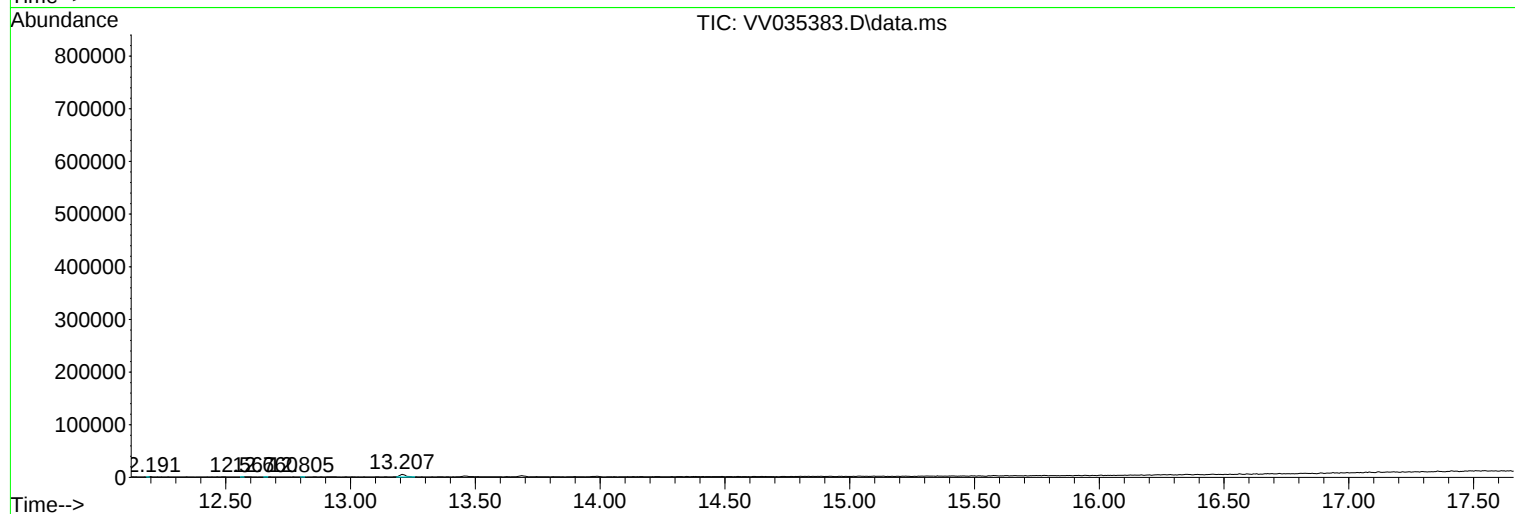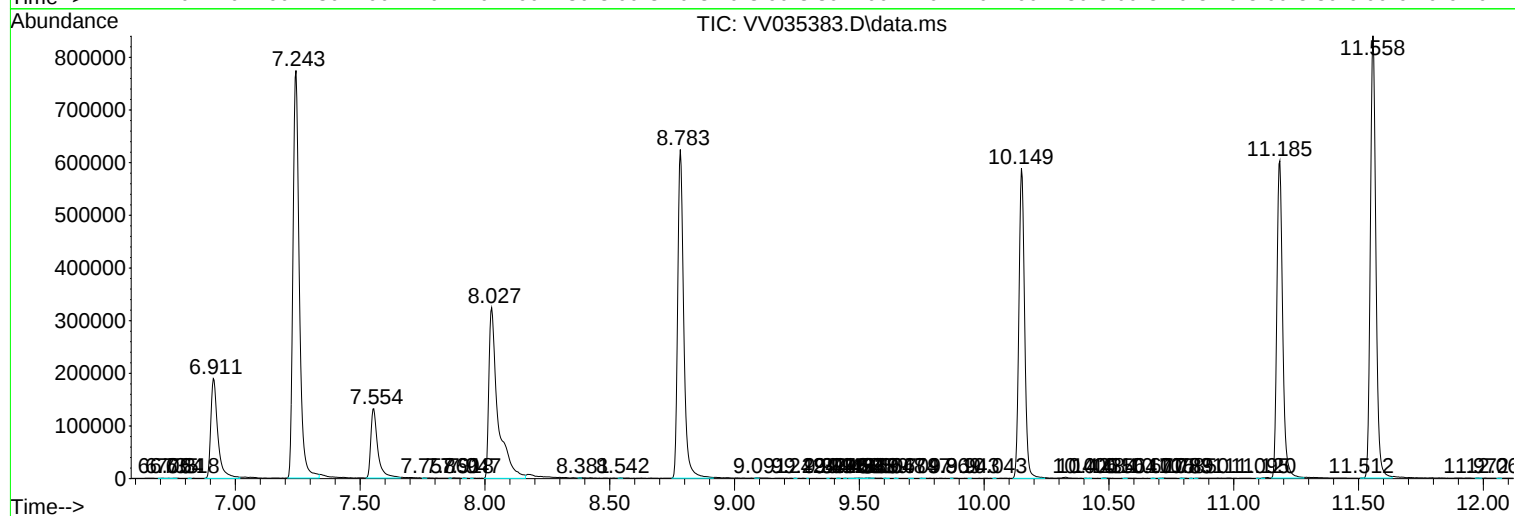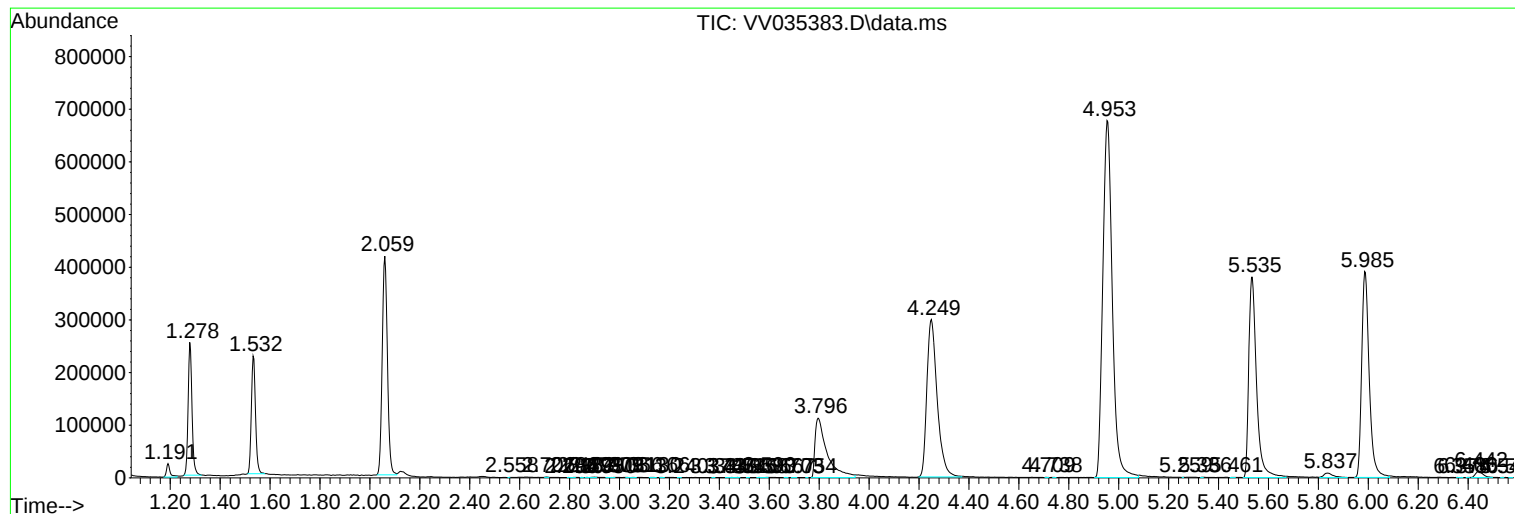

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035383.D
Acq On : 24 Apr 2024 13:38
Operator : SY/MD
Sample : P2235-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035383.D
Acq On : 24 Apr 2024 13:38
Operator : SY/MD
Sample : P2235-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08N9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------