

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035384.D
 Acq On : 24 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2238-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	229973	244121	15.02%	2.126%
2	1.532	146	153	168	rVB	201379	232668	14.31%	2.026%
3	2.060	307	317	332	rBV	376751	548811	33.77%	4.780%
4	2.445	431	437	447	rVB8	3055	4860	0.30%	0.042%
5	2.580	475	479	485	rBV2	463	615	0.04%	0.005%
6	2.722	521	523	527	rVB2	344	171	0.01%	0.001%
7	2.793	543	545	549	rVB	333	169	0.01%	0.001%
8	2.818	549	553	560	rBV2	370	510	0.03%	0.004%
9	2.886	571	574	576	rBV2	199	140	0.01%	0.001%
10	2.947	591	593	595	rBV	407	197	0.01%	0.002%
11	3.008	609	612	617	rBV4	304	209	0.01%	0.002%
12	3.175	661	664	668	rBV2	158	158	0.01%	0.001%
13	3.243	683	685	689	rVB	266	193	0.01%	0.002%
14	3.297	699	702	705	rVB2	226	119	0.01%	0.001%
15	3.397	730	733	734	rBV	292	157	0.01%	0.001%
16	3.449	744	749	752	rBV	176	146	0.01%	0.001%
17	3.506	764	767	771	rVV	236	188	0.01%	0.002%
18	3.526	771	773	775	rVV2	324	122	0.01%	0.001%
19	3.629	800	805	807	rBV2	295	261	0.02%	0.002%
20	3.654	811	813	815	rVV2	258	126	0.01%	0.001%
21	3.670	815	818	821	rVB3	292	180	0.01%	0.002%
22	3.699	824	827	830	rVB2	224	154	0.01%	0.001%
23	3.738	835	839	844	rBV3	154	157	0.01%	0.001%
24	3.760	844	846	849	rVB2	262	143	0.01%	0.001%
25	3.799	849	858	891	rBV	99195	317364	19.53%	2.764%
26	4.249	982	998	1029	rBV	257029	669502	41.19%	5.831%
27	4.622	1110	1114	1115	rBV2	471	284	0.02%	0.002%
28	4.664	1123	1127	1132	rBV2	320	309	0.02%	0.003%
29	4.780	1160	1163	1164	rBV2	205	115	0.01%	0.001%
30	4.793	1165	1167	1169	rVV	249	126	0.01%	0.001%
31	4.866	1185	1190	1193	rBV2	284	322	0.02%	0.003%
32	4.957	1202	1218	1259	rBV2	612847	1625360	100.00%	14.156%
33	5.375	1346	1348	1354	rVB2	419	301	0.02%	0.003%
34	5.403	1355	1357	1359	rBV3	285	143	0.01%	0.001%
35	5.420	1359	1362	1365	rBV2	371	230	0.01%	0.002%
36	5.471	1375	1378	1383	rBV4	486	480	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035384.D
 Acq On : 24 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2238-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.535	1387	1398	1430	rBV	345041	734441	45.19%	6.397%
38	5.934	1520	1522	1525	rBV3	276	187	0.01%	0.002%
39	5.985	1525	1538	1563	rBV	350399	738448	45.43%	6.431%
40	6.362	1652	1655	1657	rBV2	412	267	0.02%	0.002%
41	6.400	1663	1667	1669	rBV	385	234	0.01%	0.002%
42	6.413	1669	1671	1674	rVV	494	225	0.01%	0.002%
43	6.429	1674	1676	1679	rVV	222	112	0.01%	0.001%
44	6.471	1686	1689	1695	rVB4	447	411	0.03%	0.004%
45	6.619	1730	1735	1736	rBV2	263	179	0.01%	0.002%
46	6.638	1736	1741	1743	rBV3	340	276	0.02%	0.002%
47	6.667	1748	1750	1752	rBV3	261	153	0.01%	0.001%
48	6.699	1758	1760	1765	rVB2	242	146	0.01%	0.001%
49	6.776	1780	1784	1789	rVB2	296	215	0.01%	0.002%
50	6.915	1815	1827	1856	rBV	166680	329935	20.30%	2.874%
51	7.243	1918	1929	1955	rBV	691961	1216739	74.86%	10.597%
52	7.554	2017	2026	2059	rBV	117464	221916	13.65%	1.933%
53	7.953	2147	2150	2154	rBV3	288	268	0.02%	0.002%
54	7.972	2154	2156	2157	rBV	352	131	0.01%	0.001%
55	8.027	2162	2173	2225	rBV3	287702	726318	44.69%	6.326%
56	8.551	2334	2336	2338	rBV	309	182	0.01%	0.002%
57	8.587	2345	2347	2351	rVB2	424	252	0.02%	0.002%
58	8.612	2352	2355	2359	rBV3	540	496	0.03%	0.004%
59	8.783	2396	2408	2438	rBV	561986	941307	57.91%	8.198%
60	9.165	2524	2527	2529	rBV2	322	179	0.01%	0.002%
61	9.191	2532	2535	2538	rVV	347	275	0.02%	0.002%
62	9.223	2542	2545	2547	rVV2	392	240	0.01%	0.002%
63	9.300	2566	2569	2572	rVB2	320	241	0.01%	0.002%
64	9.374	2590	2592	2594	rBV2	181	106	0.01%	0.001%
65	9.561	2645	2650	2654	rBV2	464	434	0.03%	0.004%
66	9.587	2655	2658	2661	rVV2	237	179	0.01%	0.002%
67	9.728	2696	2702	2703	rBV	141	126	0.01%	0.001%
68	9.796	2717	2723	2726	rBV2	334	310	0.02%	0.003%
69	9.831	2731	2734	2737	rVB	270	181	0.01%	0.002%
70	9.905	2753	2757	2760	rBV	309	267	0.02%	0.002%
71	9.947	2768	2770	2774	rBV	171	112	0.01%	0.001%
72	10.069	2806	2808	2811	rVB	256	131	0.01%	0.001%
73	10.149	2821	2833	2860	rBV	531353	842773	51.85%	7.340%
74	10.323	2879	2887	2895	rBV7	2204	3462	0.21%	0.030%
75	10.403	2908	2912	2913	rBV	271	190	0.01%	0.002%
76	10.426	2917	2919	2922	rVV	247	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035384.D
 Acq On : 24 Apr 2024 14:01
 Operator : SY/MD
 Sample : P2238-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.493	2938	2940	2943	rVB	505	253	0.02%	0.002%
78	10.513	2943	2946	2949	rBV2	290	162	0.01%	0.001%
79	10.561	2958	2961	2966	rBV	272	182	0.01%	0.002%
80	10.619	2976	2979	2981	rBV2	253	178	0.01%	0.002%
81	10.722	3009	3011	3014	rBV2	247	146	0.01%	0.001%
82	10.757	3019	3022	3025	rBV	257	185	0.01%	0.002%
83	10.821	3038	3042	3044	rBV	163	129	0.01%	0.001%
84	11.024	3099	3105	3106	rBV	293	224	0.01%	0.002%
85	11.133	3130	3139	3144	rBV4	921	1475	0.09%	0.013%
86	11.185	3144	3155	3186	rVV	538128	867655	53.38%	7.557%
87	11.506	3246	3255	3260	rBV7	5080	9183	0.56%	0.080%
88	11.558	3261	3271	3301	rVB	753378	1179159	72.55%	10.270%
89	11.789	3339	3343	3346	rBV4	676	725	0.04%	0.006%
90	11.918	3379	3383	3384	rBV2	394	232	0.01%	0.002%
91	12.004	3406	3410	3414	rBV2	503	388	0.02%	0.003%
92	12.123	3444	3447	3452	rBV3	324	323	0.02%	0.003%
93	12.143	3452	3453	3455	rBV2	402	192	0.01%	0.002%
94	12.271	3491	3493	3497	rBV	355	193	0.01%	0.002%
95	12.291	3497	3499	3504	rVB	308	134	0.01%	0.001%
96	12.493	3560	3562	3563	rBV	290	121	0.01%	0.001%
97	12.773	3647	3649	3652	rBV2	358	225	0.01%	0.002%
98	13.207	3778	3784	3795	rVB4	3630	5306	0.33%	0.046%
99	13.294	3809	3811	3815	rBV	389	248	0.02%	0.002%
100	13.458	3853	3862	3874	rBV2	1711	3492	0.21%	0.030%




Sum of corrected areas: 11481796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035384.D
Acq On : 24 Apr 2024 14:01
Operator : SY/MD
Sample : P2238-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

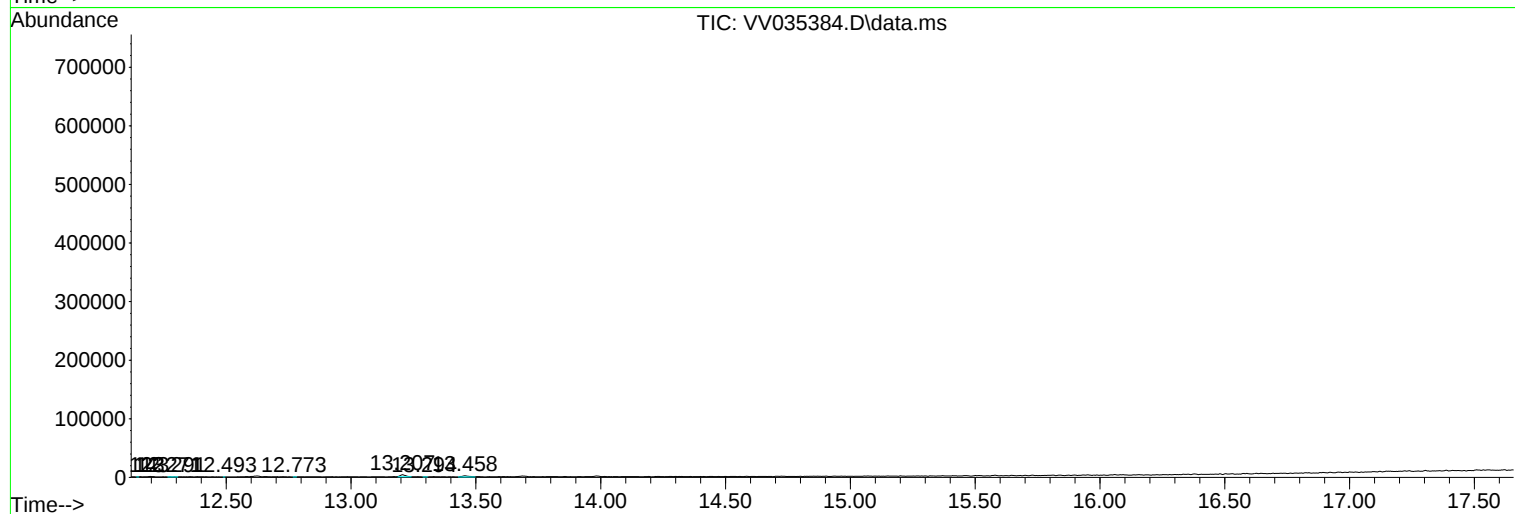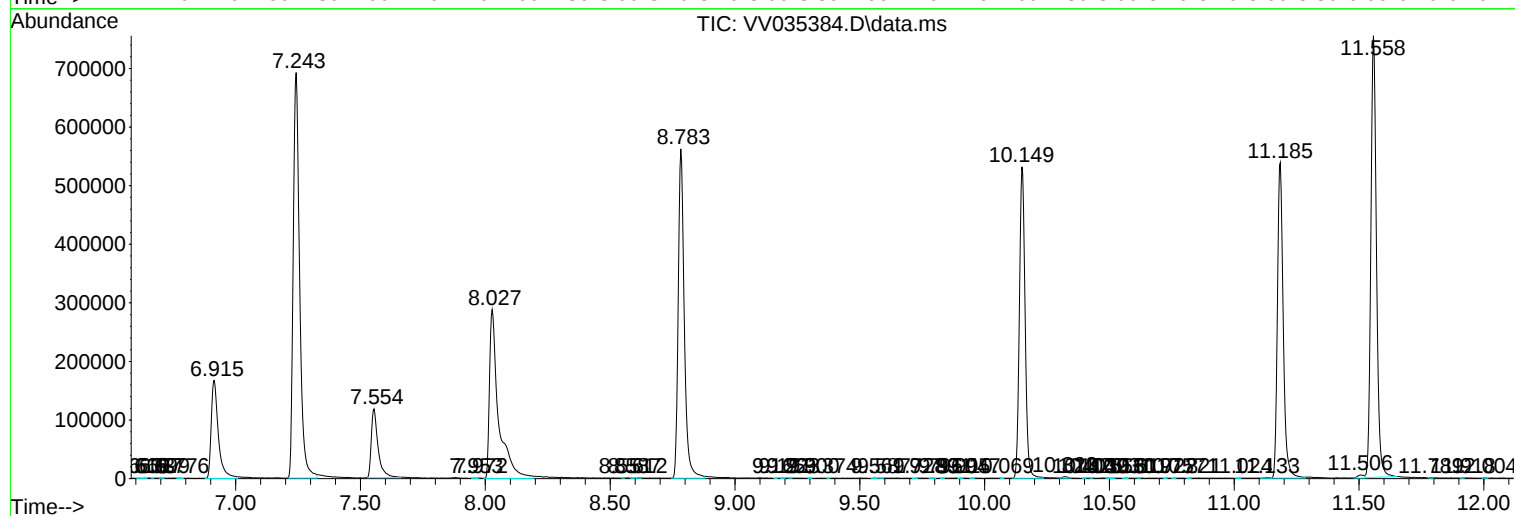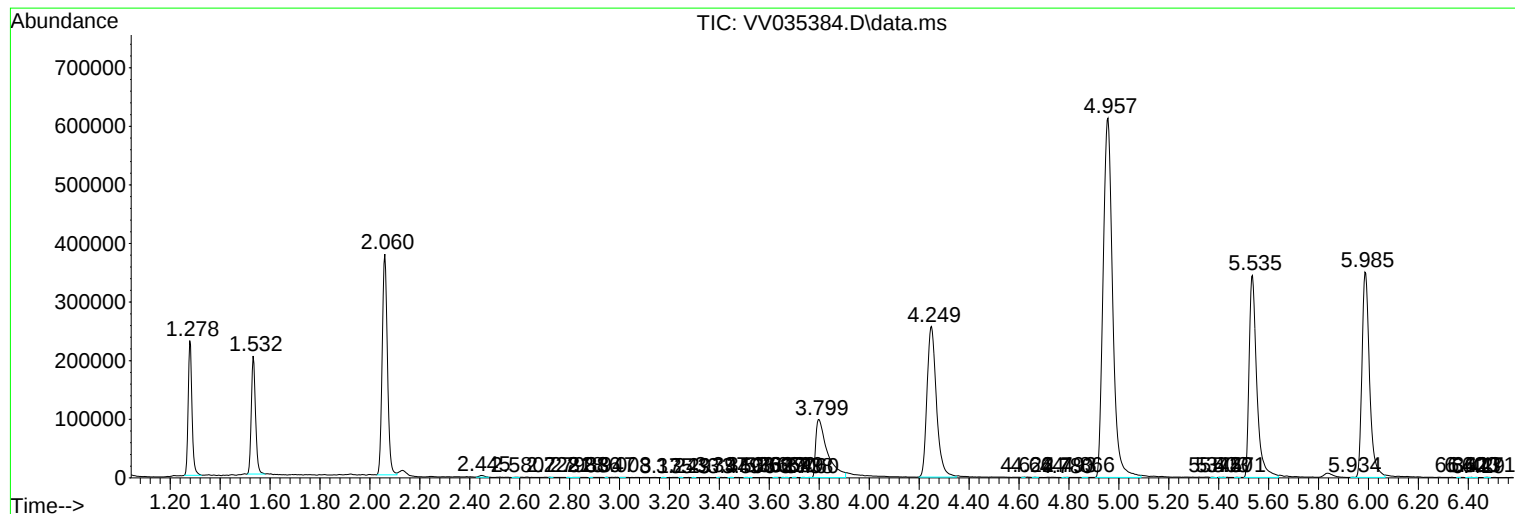

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035384.D
Acq On : 24 Apr 2024 14:01
Operator : SY/MD
Sample : P2238-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035384.D
Acq On : 24 Apr 2024 14:01
Operator : SY/MD
Sample : P2238-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CZ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
