

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035385.D
 Acq On : 24 Apr 2024 14:25
 Operator : SY/MD
 Sample : P2238-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rBV	247555	264633	15.14%	2.078%
2	1.532	146	153	166	rBV	218894	249970	14.30%	1.963%
3	2.060	307	317	331	rBV	401930	588005	33.63%	4.617%
4	2.548	467	469	473	rVB2	438	256	0.01%	0.002%
5	2.568	473	475	481	rVB3	399	393	0.02%	0.003%
6	2.593	481	483	486	rBV	325	171	0.01%	0.001%
7	2.622	486	492	495	rBV2	545	546	0.03%	0.004%
8	2.735	525	527	529	rBV	254	121	0.01%	0.001%
9	2.876	568	571	573	rBV2	345	231	0.01%	0.002%
10	2.909	579	581	584	rBV3	243	132	0.01%	0.001%
11	2.947	591	593	594	rBV3	232	85	0.00%	0.001%
12	3.028	616	618	621	rVB2	296	147	0.01%	0.001%
13	3.140	650	653	657	rVB3	178	154	0.01%	0.001%
14	3.198	668	671	676	rVB3	260	230	0.01%	0.002%
15	3.253	683	688	689	rBV	214	136	0.01%	0.001%
16	3.262	689	691	699	rVB2	333	328	0.02%	0.003%
17	3.298	699	702	707	rBV2	128	83	0.00%	0.001%
18	3.333	707	713	717	rBV	374	379	0.02%	0.003%
19	3.378	724	727	730	rBV	226	117	0.01%	0.001%
20	3.661	812	815	818	rVB2	344	232	0.01%	0.002%
21	3.696	823	826	830	rBV2	210	167	0.01%	0.001%
22	3.745	837	841	847	rBV2	194	225	0.01%	0.002%
23	3.796	848	857	891	rBV	108461	341877	19.55%	2.684%
24	4.246	983	997	1029	rBV2	277851	719243	41.14%	5.648%
25	4.748	1152	1153	1156	rVB	382	121	0.01%	0.001%
26	4.783	1162	1164	1166	rBV	201	121	0.01%	0.001%
27	4.825	1172	1177	1178	rBV2	309	280	0.02%	0.002%
28	4.873	1189	1192	1194	rBV2	248	154	0.01%	0.001%
29	4.953	1201	1217	1254	rBV2	659174	1748381	100.00%	13.729%
30	5.532	1386	1397	1434	rBV	419148	897193	51.32%	7.045%
31	5.928	1517	1520	1522	rBV2	570	327	0.02%	0.003%
32	5.986	1525	1538	1567	rBV	383012	802164	45.88%	6.299%
33	6.227	1611	1613	1614	rBV2	456	148	0.01%	0.001%
34	6.317	1638	1641	1646	rBV3	545	536	0.03%	0.004%
35	6.413	1666	1671	1672	rBV	427	276	0.02%	0.002%
36	6.468	1684	1688	1689	rBV	321	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035385.D
 Acq On : 24 Apr 2024 14:25
 Operator : SY/MD
 Sample : P2238-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.574	1718	1721	1725	rVB2	351	256	0.01%	0.002%
38	6.622	1733	1736	1737	rBV	258	114	0.01%	0.001%
39	6.664	1741	1749	1753	rBV5	504	638	0.04%	0.005%
40	6.699	1758	1760	1764	rVB2	381	175	0.01%	0.001%
41	6.728	1764	1769	1771	rBV2	252	270	0.02%	0.002%
42	6.760	1778	1779	1786	rVB3	328	239	0.01%	0.002%
43	6.796	1786	1790	1794	rBV2	286	195	0.01%	0.002%
44	6.818	1794	1797	1799	rVB	181	99	0.01%	0.001%
45	6.912	1816	1826	1859	rBV	181215	357915	20.47%	2.810%
46	7.153	1895	1901	1904	rBV3	658	694	0.04%	0.005%
47	7.243	1918	1929	1967	rBV	737894	1320606	75.53%	10.370%
48	7.519	2013	2015	2016	rBV	450	186	0.01%	0.001%
49	7.551	2016	2025	2061	rVV2	126551	247924	14.18%	1.947%
50	7.796	2099	2101	2102	rBV2	293	115	0.01%	0.001%
51	7.825	2107	2110	2113	rBV2	312	290	0.02%	0.002%
52	7.870	2118	2124	2125	rBV2	845	704	0.04%	0.006%
53	7.973	2153	2156	2161	rBV2	484	387	0.02%	0.003%
54	8.027	2161	2173	2219	rBV2	311893	779989	44.61%	6.125%
55	8.513	2320	2324	2325	rBV2	370	201	0.01%	0.002%
56	8.658	2367	2369	2371	rBV2	271	172	0.01%	0.001%
57	8.783	2397	2408	2435	rBV	684471	1141637	65.30%	8.964%
58	9.082	2498	2501	2507	rBV4	708	592	0.03%	0.005%
59	9.146	2518	2521	2524	rBV2	411	300	0.02%	0.002%
60	9.227	2542	2546	2548	rBV2	281	233	0.01%	0.002%
61	9.278	2559	2562	2564	rBV	248	193	0.01%	0.002%
62	9.301	2567	2569	2571	rBV	299	185	0.01%	0.001%
63	9.310	2571	2572	2574	rVV	369	136	0.01%	0.001%
64	9.339	2577	2581	2584	rVB3	340	212	0.01%	0.002%
65	9.358	2585	2587	2588	rBV3	243	92	0.01%	0.001%
66	9.416	2602	2605	2610	rVB3	375	327	0.02%	0.003%
67	9.448	2611	2615	2617	rVB2	197	101	0.01%	0.001%
68	9.468	2617	2621	2623	rBV2	351	237	0.01%	0.002%
69	9.503	2630	2632	2638	rVB4	595	597	0.03%	0.005%
70	9.625	2666	2670	2671	rBV	310	187	0.01%	0.001%
71	9.683	2686	2688	2693	rBV2	282	185	0.01%	0.001%
72	9.754	2708	2710	2713	rVB2	253	124	0.01%	0.001%
73	9.812	2725	2728	2732	rBV2	448	284	0.02%	0.002%
74	9.924	2760	2763	2766	rBV2	233	106	0.01%	0.001%
75	10.008	2785	2789	2790	rBV2	217	142	0.01%	0.001%
76	10.056	2802	2804	2805	rBV	243	93	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035385.D
 Acq On : 24 Apr 2024 14:25
 Operator : SY/MD
 Sample : P2238-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.095	2811	2816	2817	rBV2	200	149	0.01%	0.001%
78	10.149	2822	2833	2863	rVV	570526	904432	51.73%	7.102%
79	10.426	2917	2919	2921	rVB2	310	154	0.01%	0.001%
80	10.442	2921	2924	2925	rBV	240	126	0.01%	0.001%
81	10.471	2929	2933	2937	rBV3	702	662	0.04%	0.005%
82	10.545	2951	2956	2958	rBV2	280	242	0.01%	0.002%
83	10.696	3000	3003	3007	rBV	206	139	0.01%	0.001%
84	10.722	3007	3011	3013	rVB	314	198	0.01%	0.002%
85	10.747	3016	3019	3021	rBV	197	144	0.01%	0.001%
86	10.796	3032	3034	3035	rBV	255	119	0.01%	0.001%
87	10.873	3055	3058	3059	rBV	402	190	0.01%	0.001%
88	10.995	3094	3096	3100	rBV2	266	186	0.01%	0.001%
89	11.095	3124	3127	3129	rBV2	363	223	0.01%	0.002%
90	11.130	3133	3138	3144	rBV5	968	1437	0.08%	0.011%
91	11.185	3144	3155	3181	rBV	671051	1059885	60.62%	8.322%
92	11.503	3246	3254	3259	rBV6	6660	11143	0.64%	0.087%
93	11.558	3261	3271	3295	rVB	810228	1275294	72.94%	10.014%
94	12.185	3461	3466	3467	rBV	483	460	0.03%	0.004%
95	12.313	3502	3506	3509	rBV3	781	712	0.04%	0.006%
96	12.481	3555	3558	3563	rBV2	369	355	0.02%	0.003%
97	12.583	3588	3590	3591	rBV	379	134	0.01%	0.001%
98	12.731	3633	3636	3642	rBV2	414	341	0.02%	0.003%
99	12.927	3695	3697	3701	rBV2	198	135	0.01%	0.001%
100	13.207	3779	3784	3791	rBV5	2637	3611	0.21%	0.028%




Sum of corrected areas: 12735331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035385.D
Acq On : 24 Apr 2024 14:25
Operator : SY/MD
Sample : P2238-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

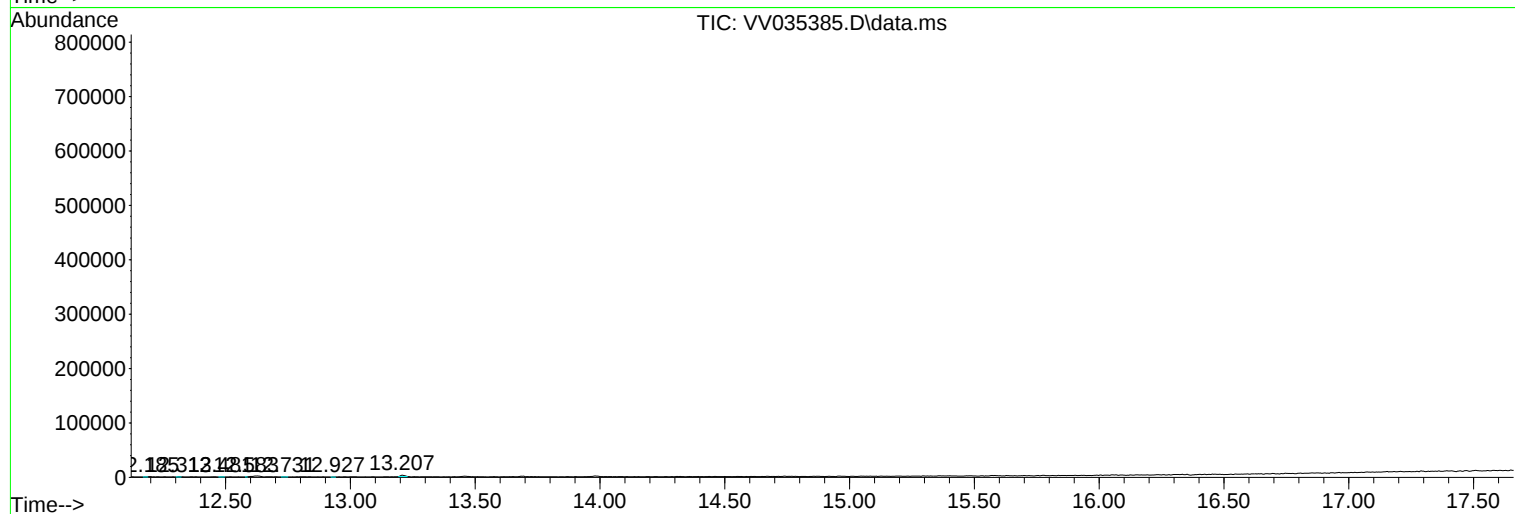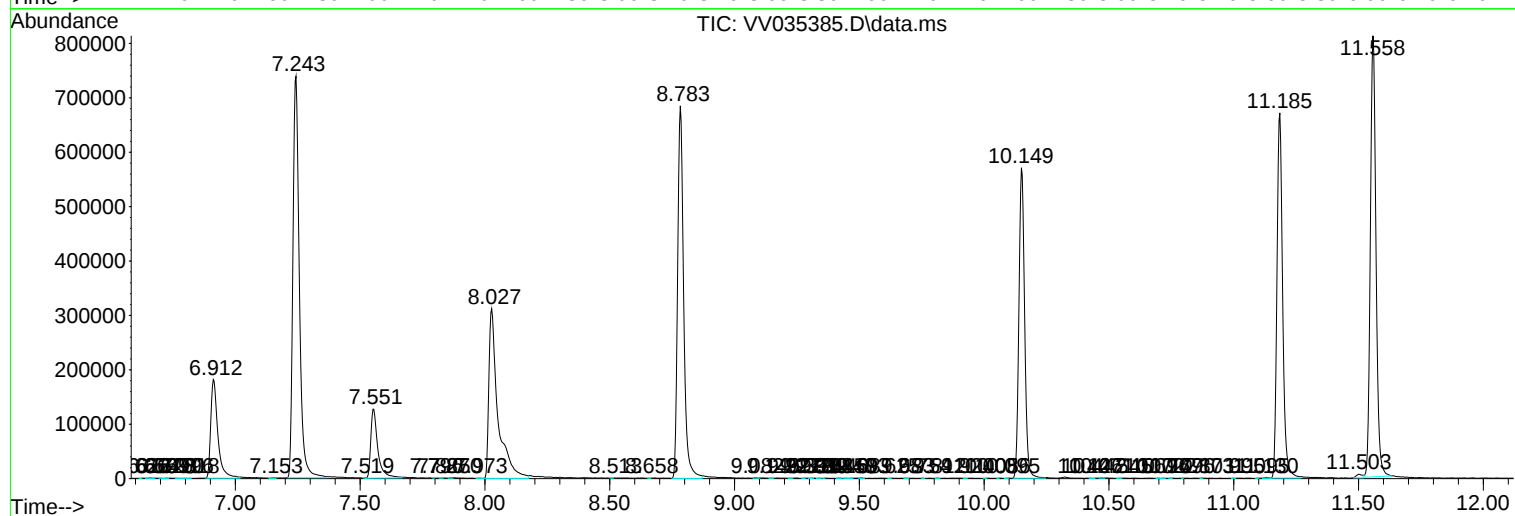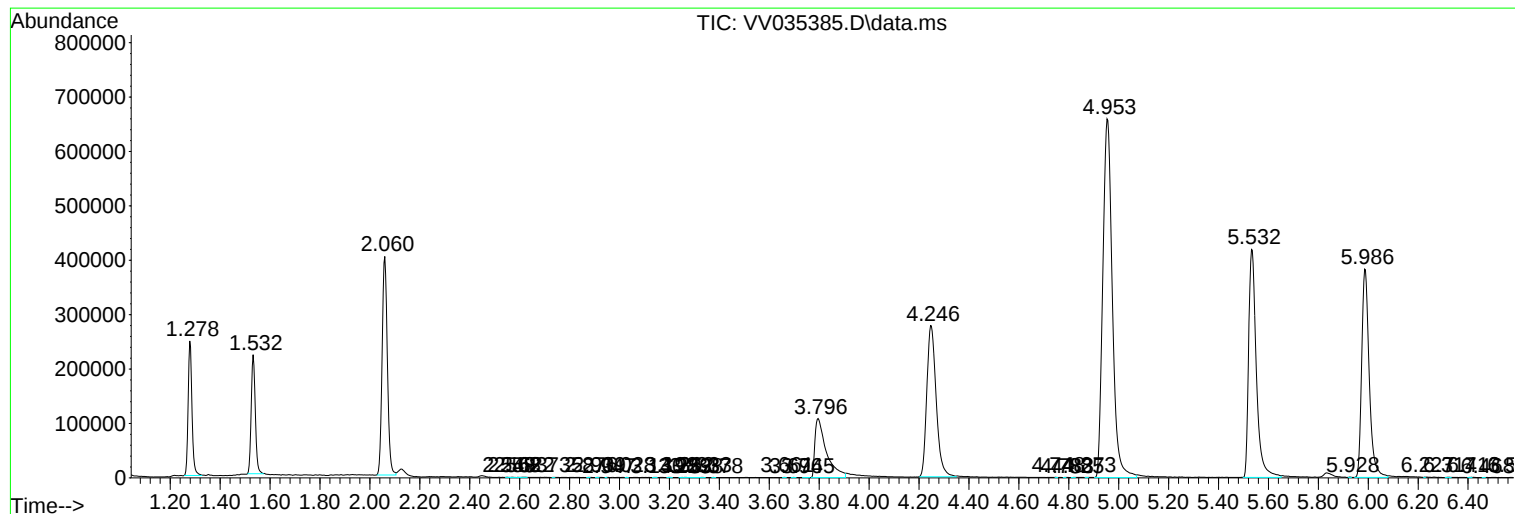

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035385.D
Acq On : 24 Apr 2024 14:25
Operator : SY/MD
Sample : P2238-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035385.D
Acq On : 24 Apr 2024 14:25
Operator : SY/MD
Sample : P2238-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------