

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035386.D
 Acq On : 24 Apr 2024 14:48
 Operator : SY/MD
 Sample : P2238-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	92	rBV	248638	264099	14.86%	2.037%
2	1.532	146	153	166	rBV	215369	246072	13.85%	1.898%
3	2.060	307	317	331	rBV	410296	592420	33.34%	4.569%
4	2.452	431	439	447	rVB5	2945	5081	0.29%	0.039%
5	2.590	480	482	484	rBV5	325	135	0.01%	0.001%
6	2.629	493	494	497	rVB	241	93	0.01%	0.001%
7	2.674	504	508	512	rBV4	592	528	0.03%	0.004%
8	2.760	532	535	537	rBV	188	114	0.01%	0.001%
9	2.770	537	538	540	rBV	257	104	0.01%	0.001%
10	2.834	552	558	562	rBV2	426	431	0.02%	0.003%
11	2.876	569	571	573	rBV	196	94	0.01%	0.001%
12	2.969	598	600	604	rVB2	258	130	0.01%	0.001%
13	3.082	632	635	640	rVB	365	195	0.01%	0.002%
14	3.169	659	662	665	rVV2	268	183	0.01%	0.001%
15	3.185	665	667	669	rVV2	129	59	0.00%	0.000%
16	3.265	688	692	696	rBV2	217	264	0.01%	0.002%
17	3.320	706	709	714	rBV2	186	202	0.01%	0.002%
18	3.352	714	719	723	rBV3	234	314	0.02%	0.002%
19	3.468	751	755	757	rBV	254	150	0.01%	0.001%
20	3.487	757	761	766	rVV2	280	333	0.02%	0.003%
21	3.519	769	771	773	rVV2	186	63	0.00%	0.000%
22	3.542	776	778	781	rBV	89	57	0.00%	0.000%
23	3.587	789	792	793	rBV	232	136	0.01%	0.001%
24	3.641	806	809	815	rVB	242	183	0.01%	0.001%
25	3.667	815	817	819	rBV2	160	100	0.01%	0.001%
26	3.703	824	828	833	rBV2	270	260	0.01%	0.002%
27	3.725	833	835	837	rBV2	112	51	0.00%	0.000%
28	3.796	848	857	900	rBV	109313	357068	20.10%	2.754%
29	4.246	983	997	1030	rBV	278492	721624	40.61%	5.565%
30	4.619	1109	1113	1116	rBV3	551	500	0.03%	0.004%
31	4.870	1187	1191	1197	rVB2	444	433	0.02%	0.003%
32	4.953	1197	1217	1271	rBV2	664680	1776818	100.00%	13.704%
33	5.310	1326	1328	1330	rBV	307	176	0.01%	0.001%
34	5.532	1387	1397	1435	rBV	435411	928839	52.28%	7.164%
35	5.838	1482	1492	1507	rBV3	8840	20052	1.13%	0.155%
36	5.918	1515	1517	1519	rBV	262	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035386.D
 Acq On : 24 Apr 2024 14:48
 Operator : SY/MD
 Sample : P2238-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.985	1526	1538	1575	rBV	386639	808821	45.52%	6.238%
38	6.310	1635	1639	1643	rVB3	423	362	0.02%	0.003%
39	6.339	1645	1648	1649	rBV2	307	181	0.01%	0.001%
40	6.384	1659	1662	1667	rVB2	363	297	0.02%	0.002%
41	6.410	1667	1670	1671	rBV	174	114	0.01%	0.001%
42	6.448	1679	1682	1686	rBV2	210	142	0.01%	0.001%
43	6.481	1686	1692	1696	rBV	165	139	0.01%	0.001%
44	6.500	1696	1698	1701	rBV2	282	180	0.01%	0.001%
45	6.516	1701	1703	1704	rBV	140	47	0.00%	0.000%
46	6.625	1734	1737	1742	rBV3	345	356	0.02%	0.003%
47	6.648	1742	1744	1747	rVB	289	158	0.01%	0.001%
48	6.674	1748	1752	1753	rBV2	274	190	0.01%	0.001%
49	6.709	1761	1763	1767	rBV2	267	213	0.01%	0.002%
50	6.731	1767	1770	1775	rBV2	376	380	0.02%	0.003%
51	6.754	1775	1777	1781	rVV2	277	146	0.01%	0.001%
52	6.805	1791	1793	1800	rVB	440	261	0.01%	0.002%
53	6.837	1800	1803	1806	rBV	235	137	0.01%	0.001%
54	6.863	1809	1811	1816	rVB2	233	161	0.01%	0.001%
55	6.911	1816	1826	1867	rBV	183162	363090	20.43%	2.800%
56	7.165	1903	1905	1909	rBV2	567	472	0.03%	0.004%
57	7.243	1917	1929	1956	rBV	752119	1334867	75.13%	10.295%
58	7.551	2017	2025	2054	rBV	129567	240969	13.56%	1.858%
59	7.879	2120	2127	2134	rVV4	996	1672	0.09%	0.013%
60	7.921	2138	2140	2150	rBV4	672	663	0.04%	0.005%
61	7.973	2155	2156	2158	rBV4	161	51	0.00%	0.000%
62	7.985	2158	2160	2163	rBB	299	130	0.01%	0.001%
63	8.027	2163	2173	2224	rBV3	311221	786065	44.24%	6.062%
64	8.783	2397	2408	2447	rBV	697825	1179663	66.39%	9.098%
65	9.153	2520	2523	2525	rBV3	292	227	0.01%	0.002%
66	9.185	2531	2533	2536	rVB3	353	119	0.01%	0.001%
67	9.201	2536	2538	2539	rBV	429	174	0.01%	0.001%
68	9.294	2563	2567	2574	rBV2	275	326	0.02%	0.003%
69	9.326	2574	2577	2580	rBV	430	243	0.01%	0.002%
70	9.394	2596	2598	2601	rBV2	165	92	0.01%	0.001%
71	9.474	2621	2623	2624	rBV2	147	49	0.00%	0.000%
72	9.564	2647	2651	2652	rBV	218	156	0.01%	0.001%
73	9.609	2662	2665	2666	rBV	140	79	0.00%	0.001%
74	9.632	2670	2672	2675	rVV2	203	120	0.01%	0.001%
75	9.670	2681	2684	2685	rBV	289	167	0.01%	0.001%
76	9.763	2709	2713	2716	rBV2	294	285	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035386.D
 Acq On : 24 Apr 2024 14:48
 Operator : SY/MD
 Sample : P2238-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1D16

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.834	2731	2735	2736	rBV	260	174	0.01%	0.001%
78	9.857	2740	2742	2745	rBV2	185	143	0.01%	0.001%
79	9.905	2755	2757	2760	rBV2	166	99	0.01%	0.001%
80	10.043	2796	2800	2804	rVB2	355	251	0.01%	0.002%
81	10.062	2804	2806	2808	rBV2	163	102	0.01%	0.001%
82	10.149	2822	2833	2862	rBV	577286	909263	51.17%	7.013%
83	10.374	2898	2903	2904	rBV	454	344	0.02%	0.003%
84	10.432	2918	2921	2925	rVB	410	274	0.02%	0.002%
85	10.471	2927	2933	2941	rBV6	741	1071	0.06%	0.008%
86	10.506	2941	2944	2948	rBV2	283	220	0.01%	0.002%
87	10.596	2970	2972	2974	rBV	241	97	0.01%	0.001%
88	10.628	2980	2982	2985	rVB2	246	123	0.01%	0.001%
89	10.644	2985	2987	2989	rBV2	199	112	0.01%	0.001%
90	10.924	3072	3074	3078	rVB2	337	203	0.01%	0.002%
91	11.095	3125	3127	3129	rBV	148	62	0.00%	0.000%
92	11.136	3132	3140	3143	rBV2	892	1120	0.06%	0.009%
93	11.185	3143	3155	3185	rBV	673596	1091317	61.42%	8.417%
94	11.500	3244	3253	3260	rBV2	11006	22234	1.25%	0.171%
95	11.558	3261	3271	3305	rVB	811979	1297638	73.03%	10.008%
96	11.786	3340	3342	3345	rBV3	777	453	0.03%	0.003%
97	12.017	3411	3414	3415	rBV2	448	228	0.01%	0.002%
98	12.188	3464	3467	3469	rBV2	857	631	0.04%	0.005%
99	12.397	3530	3532	3534	rBV2	398	174	0.01%	0.001%
100	12.757	3641	3644	3647	rBV2	363	238	0.01%	0.002%




Sum of corrected areas: 12966026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035386.D
Acq On : 24 Apr 2024 14:48
Operator : SY/MD
Sample : P2238-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

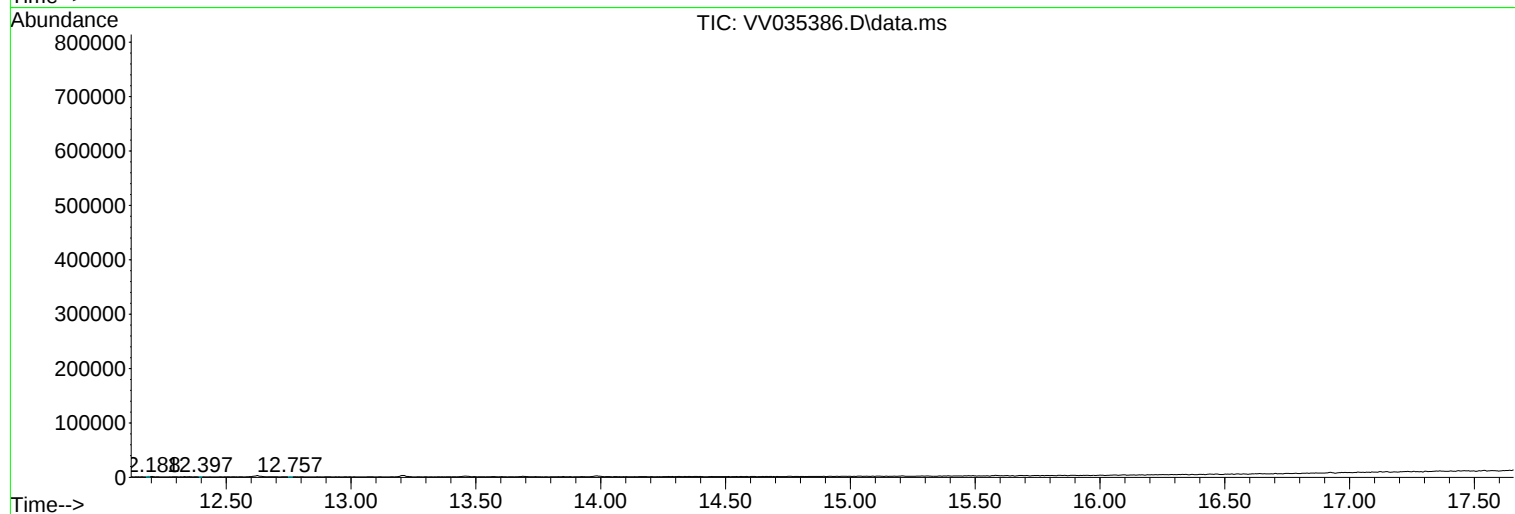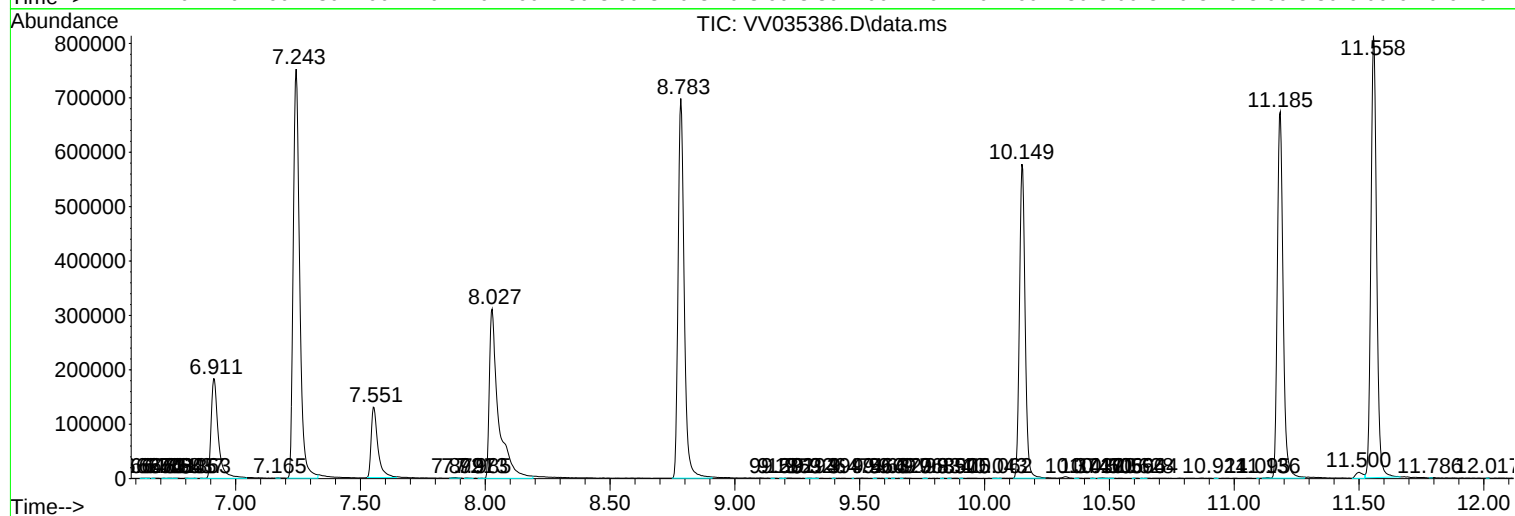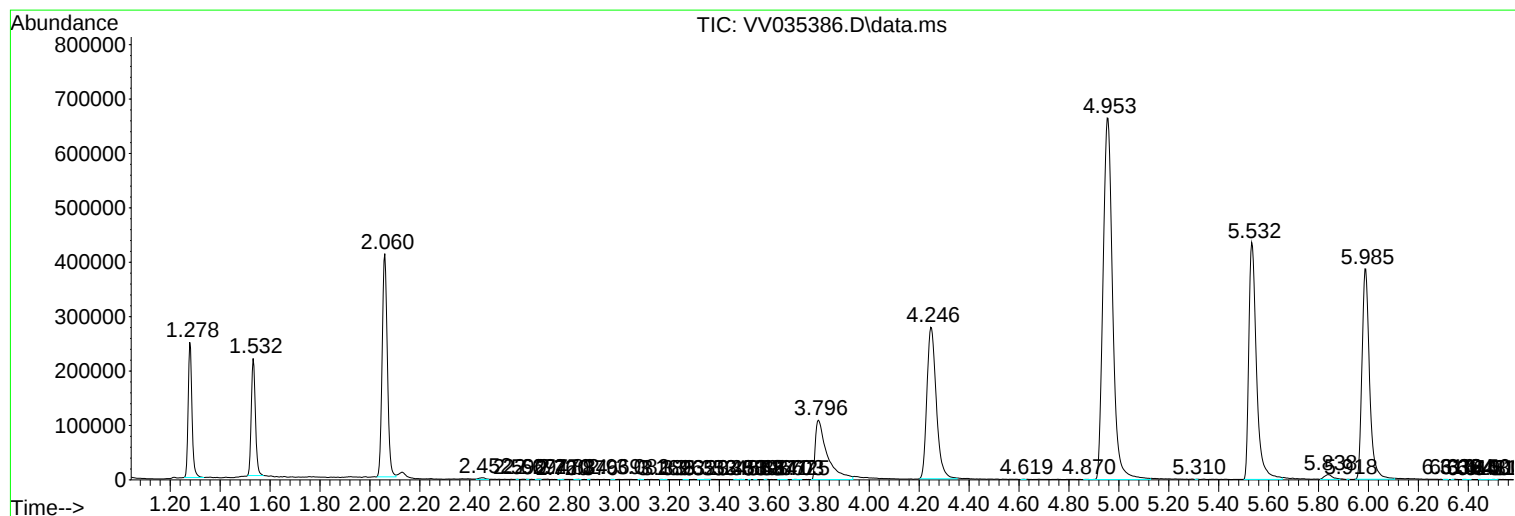

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035386.D
Acq On : 24 Apr 2024 14:48
Operator : SY/MD
Sample : P2238-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035386.D
Acq On : 24 Apr 2024 14:48
Operator : SY/MD
Sample : P2238-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1D16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc