

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035387.D
 Acq On : 24 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2164-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	246419	261094	14.75%	2.003%
2	1.532	146	153	168	rVB	220289	257142	14.52%	1.973%
3	2.060	307	317	351	rVB	412734	618265	34.92%	4.744%
4	2.600	481	485	486	rBV2	326	224	0.01%	0.002%
5	2.799	544	547	551	rBV2	247	194	0.01%	0.001%
6	2.941	588	591	593	rBV2	337	206	0.01%	0.002%
7	3.015	610	614	617	rVB2	249	179	0.01%	0.001%
8	3.108	639	643	648	rBV3	414	383	0.02%	0.003%
9	3.130	648	650	653	rBV2	207	131	0.01%	0.001%
10	3.166	658	661	663	rBV2	226	157	0.01%	0.001%
11	3.207	672	674	680	rVB2	232	159	0.01%	0.001%
12	3.243	680	685	692	rVB2	288	285	0.02%	0.002%
13	3.278	694	696	698	rBV	145	68	0.00%	0.001%
14	3.336	712	714	719	rVB	222	156	0.01%	0.001%
15	3.365	719	723	725	rBV	346	255	0.01%	0.002%
16	3.400	731	734	739	rVB2	238	154	0.01%	0.001%
17	3.426	739	742	745	rBV	255	166	0.01%	0.001%
18	3.519	769	771	774	rBV2	115	86	0.00%	0.001%
19	3.535	774	776	779	rVV3	192	112	0.01%	0.001%
20	3.551	779	781	784	rVB	124	70	0.00%	0.001%
21	3.593	793	794	801	rVB2	166	120	0.01%	0.001%
22	3.629	801	805	808	rBV3	176	144	0.01%	0.001%
23	3.645	808	810	811	rBV3	135	60	0.00%	0.000%
24	3.757	843	845	848	rBV2	185	86	0.00%	0.001%
25	3.793	848	856	899	rBV	113597	359727	20.32%	2.760%
26	4.246	981	997	1024	rBV	281434	727536	41.09%	5.582%
27	4.693	1134	1136	1138	rBV2	296	179	0.01%	0.001%
28	4.838	1178	1181	1183	rBV2	364	202	0.01%	0.002%
29	4.953	1202	1217	1253	rBV2	667199	1770683	100.00%	13.586%
30	5.448	1369	1371	1372	rBV	186	75	0.00%	0.001%
31	5.532	1387	1397	1435	rBV	445391	937494	52.95%	7.193%
32	5.838	1484	1492	1506	rVB4	7404	14654	0.83%	0.112%
33	5.989	1526	1539	1576	rBV	385877	813361	45.93%	6.241%
34	6.339	1645	1648	1649	rBV2	506	286	0.02%	0.002%
35	6.416	1669	1672	1676	rVB2	360	294	0.02%	0.002%
36	6.436	1676	1678	1679	rBV	139	35	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035387.D
 Acq On : 24 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2164-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.445	1679	1681	1683	rBV	151	57	0.00%	0.000%
38	6.461	1683	1686	1687	rBV2	190	101	0.01%	0.001%
39	6.593	1724	1727	1729	rBV2	115	76	0.00%	0.001%
40	6.606	1729	1731	1735	rBV2	327	182	0.01%	0.001%
41	6.625	1735	1737	1738	rBV	175	70	0.00%	0.001%
42	6.670	1747	1751	1754	rBV	493	394	0.02%	0.003%
43	6.715	1763	1765	1766	rBV	151	68	0.00%	0.001%
44	6.725	1766	1768	1770	rBV	210	129	0.01%	0.001%
45	6.764	1778	1780	1783	rBV2	219	110	0.01%	0.001%
46	6.812	1791	1795	1802	rBV3	383	408	0.02%	0.003%
47	6.844	1802	1805	1810	rVB	241	198	0.01%	0.002%
48	6.870	1810	1813	1816	rBV	306	208	0.01%	0.002%
49	6.911	1816	1826	1848	rBV	187327	356417	20.13%	2.735%
50	7.243	1918	1929	1970	rBV	759287	1349906	76.24%	10.358%
51	7.555	2016	2026	2057	rBV	128510	247885	14.00%	1.902%
52	7.992	2159	2162	2164	rBV2	237	186	0.01%	0.001%
53	8.027	2164	2173	2226	rBV2	326893	800324	45.20%	6.141%
54	8.526	2326	2328	2331	rVB2	635	300	0.02%	0.002%
55	8.587	2345	2347	2351	rVB2	472	295	0.02%	0.002%
56	8.690	2377	2379	2382	rVB2	244	119	0.01%	0.001%
57	8.709	2382	2385	2386	rBV2	226	140	0.01%	0.001%
58	8.783	2397	2408	2447	rBV	716370	1196427	67.57%	9.180%
59	9.124	2512	2514	2515	rBV	289	135	0.01%	0.001%
60	9.207	2538	2540	2544	rVB2	301	156	0.01%	0.001%
61	9.233	2546	2548	2553	rVB2	653	482	0.03%	0.004%
62	9.259	2553	2556	2557	rBV2	200	98	0.01%	0.001%
63	9.339	2576	2581	2582	rBV2	227	201	0.01%	0.002%
64	9.400	2597	2600	2602	rVB	187	102	0.01%	0.001%
65	9.480	2622	2625	2627	rBV	199	142	0.01%	0.001%
66	9.558	2642	2649	2653	rVB3	417	408	0.02%	0.003%
67	9.590	2657	2659	2662	rVB2	202	113	0.01%	0.001%
68	9.606	2662	2664	2665	rBV	120	46	0.00%	0.000%
69	9.638	2673	2674	2677	rVB	146	57	0.00%	0.000%
70	9.670	2679	2684	2689	rVB2	373	324	0.02%	0.002%
71	9.699	2691	2693	2695	rVV	233	98	0.01%	0.001%
72	9.741	2699	2706	2709	rBV2	212	245	0.01%	0.002%
73	9.796	2719	2723	2726	rBV2	268	203	0.01%	0.002%
74	9.828	2730	2733	2736	rBV	282	169	0.01%	0.001%
75	9.876	2745	2748	2749	rBV	395	217	0.01%	0.002%
76	9.931	2762	2765	2768	rBV2	302	194	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
 Data File : VV035387.D
 Acq On : 24 Apr 2024 15:11
 Operator : SY/MD
 Sample : P2164-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0SB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.985	2780	2782	2783	rBV2	159	63	0.00%	0.000%
78	10.014	2789	2791	2793	rVB2	299	109	0.01%	0.001%
79	10.149	2821	2833	2861	rBV	584356	920841	52.00%	7.066%
80	10.355	2895	2897	2898	rBV	301	110	0.01%	0.001%
81	10.587	2966	2969	2970	rBV	273	152	0.01%	0.001%
82	10.738	3010	3016	3019	rBV	327	393	0.02%	0.003%
83	10.792	3031	3033	3038	rVB3	757	457	0.03%	0.004%
84	10.882	3059	3061	3065	rVB2	326	179	0.01%	0.001%
85	10.927	3072	3075	3079	rBV	220	144	0.01%	0.001%
86	11.062	3114	3117	3122	rVB2	236	131	0.01%	0.001%
87	11.085	3122	3124	3126	rBV2	175	68	0.00%	0.001%
88	11.133	3132	3139	3141	rBV3	1133	1219	0.07%	0.009%
89	11.185	3144	3155	3184	rVV	684995	1101539	62.21%	8.452%
90	11.468	3239	3243	3246	rBV2	540	523	0.03%	0.004%
91	11.509	3248	3256	3259	rBV5	3784	5519	0.31%	0.042%
92	11.558	3261	3271	3293	rVV	804806	1273863	71.94%	9.774%
93	12.175	3457	3463	3464	rBV2	446	374	0.02%	0.003%
94	12.490	3559	3561	3562	rBV	288	125	0.01%	0.001%
95	12.525	3569	3572	3574	rBV	602	346	0.02%	0.003%
96	12.567	3583	3585	3588	rBV	324	234	0.01%	0.002%
97	12.583	3588	3590	3595	rVV3	601	528	0.03%	0.004%
98	13.210	3778	3785	3796	rBV5	2219	3837	0.22%	0.029%
99	13.554	3890	3892	3893	rBV	444	188	0.01%	0.001%




Sum of corrected areas: 13032754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035387.D
Acq On : 24 Apr 2024 15:11
Operator : SY/MD
Sample : P2164-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

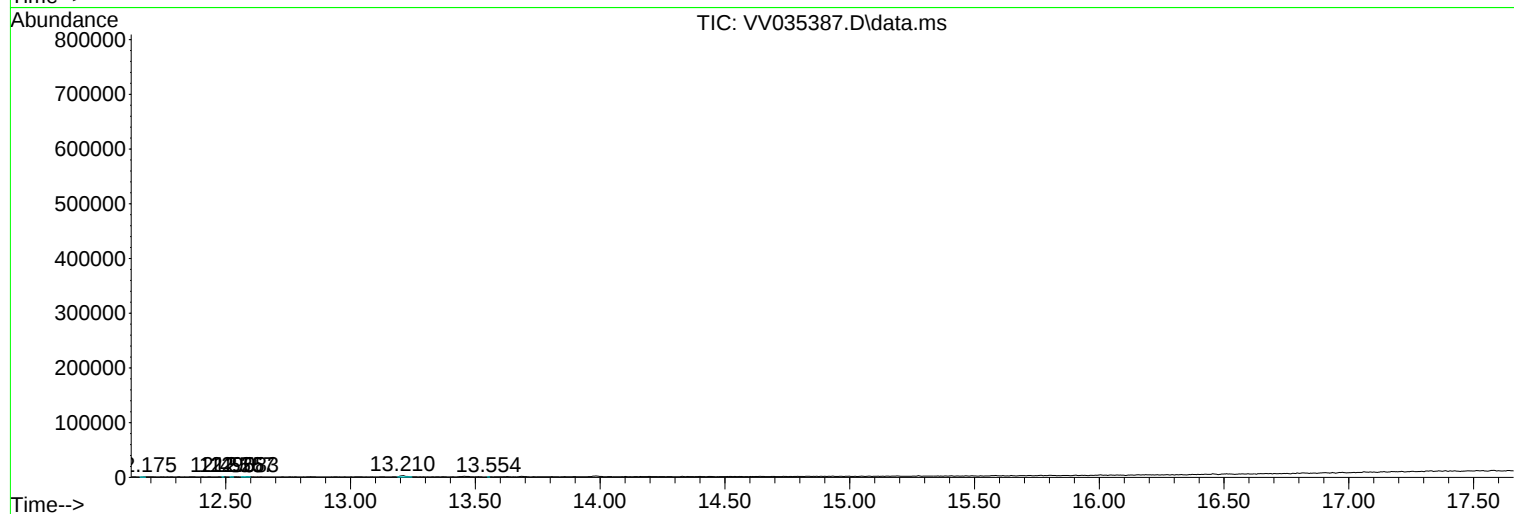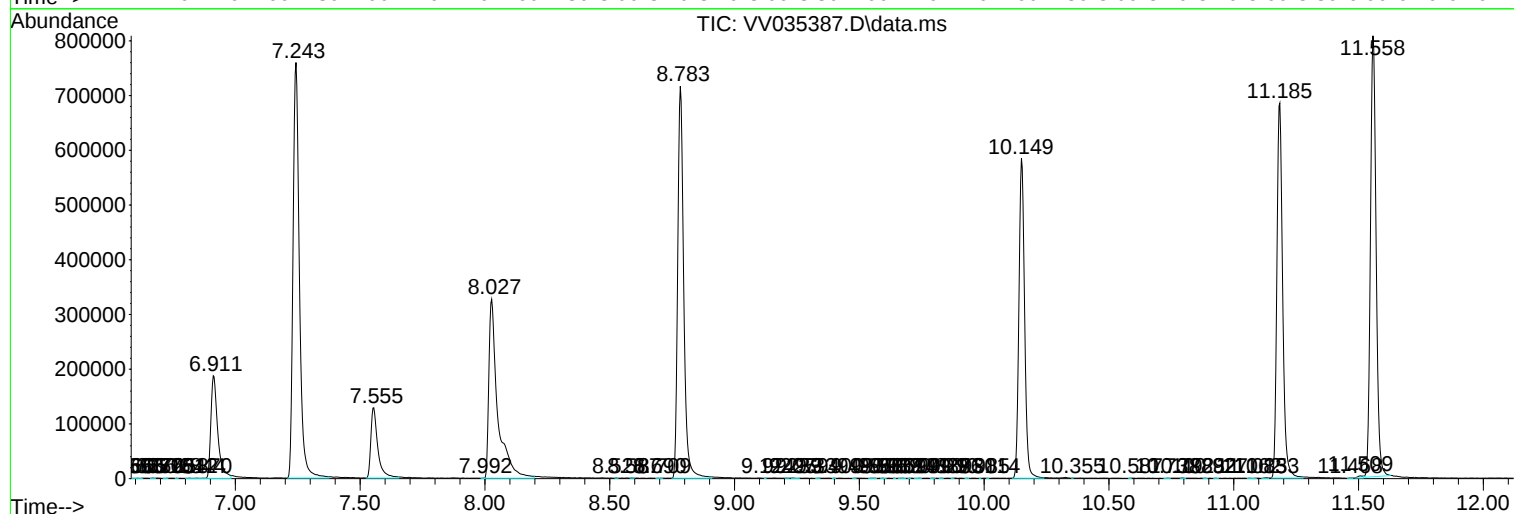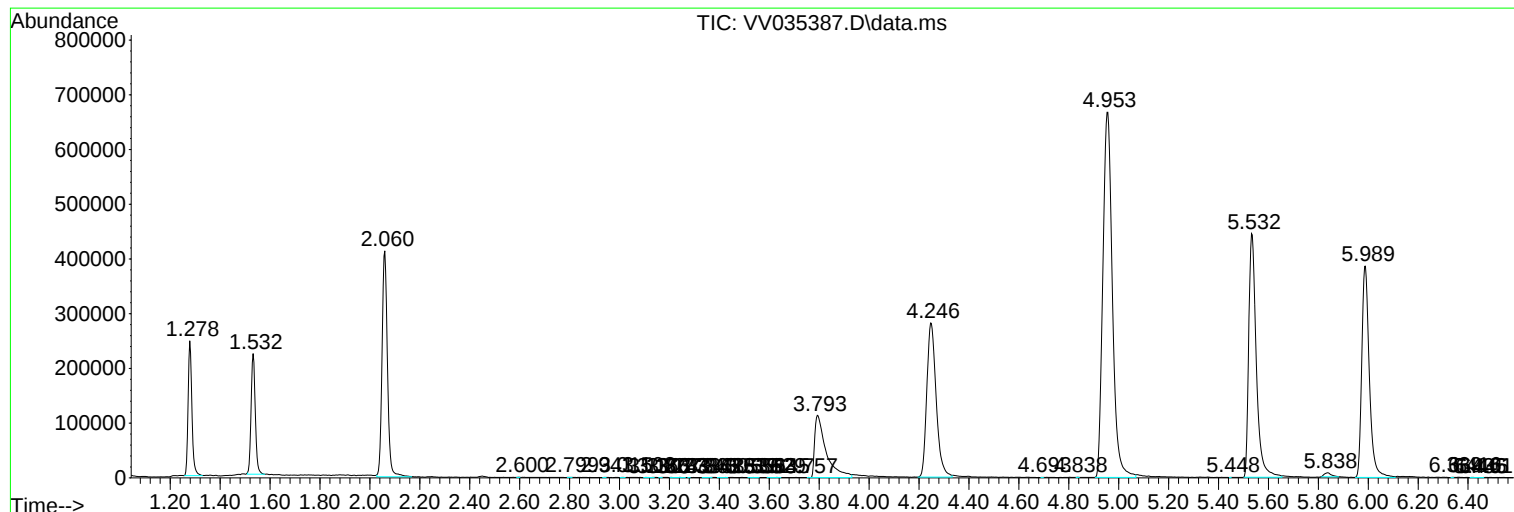

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035387.D
Acq On : 24 Apr 2024 15:11
Operator : SY/MD
Sample : P2164-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042424\
Data File : VV035387.D
Acq On : 24 Apr 2024 15:11
Operator : SY/MD
Sample : P2164-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0SB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------